




Network Analyzer Basics

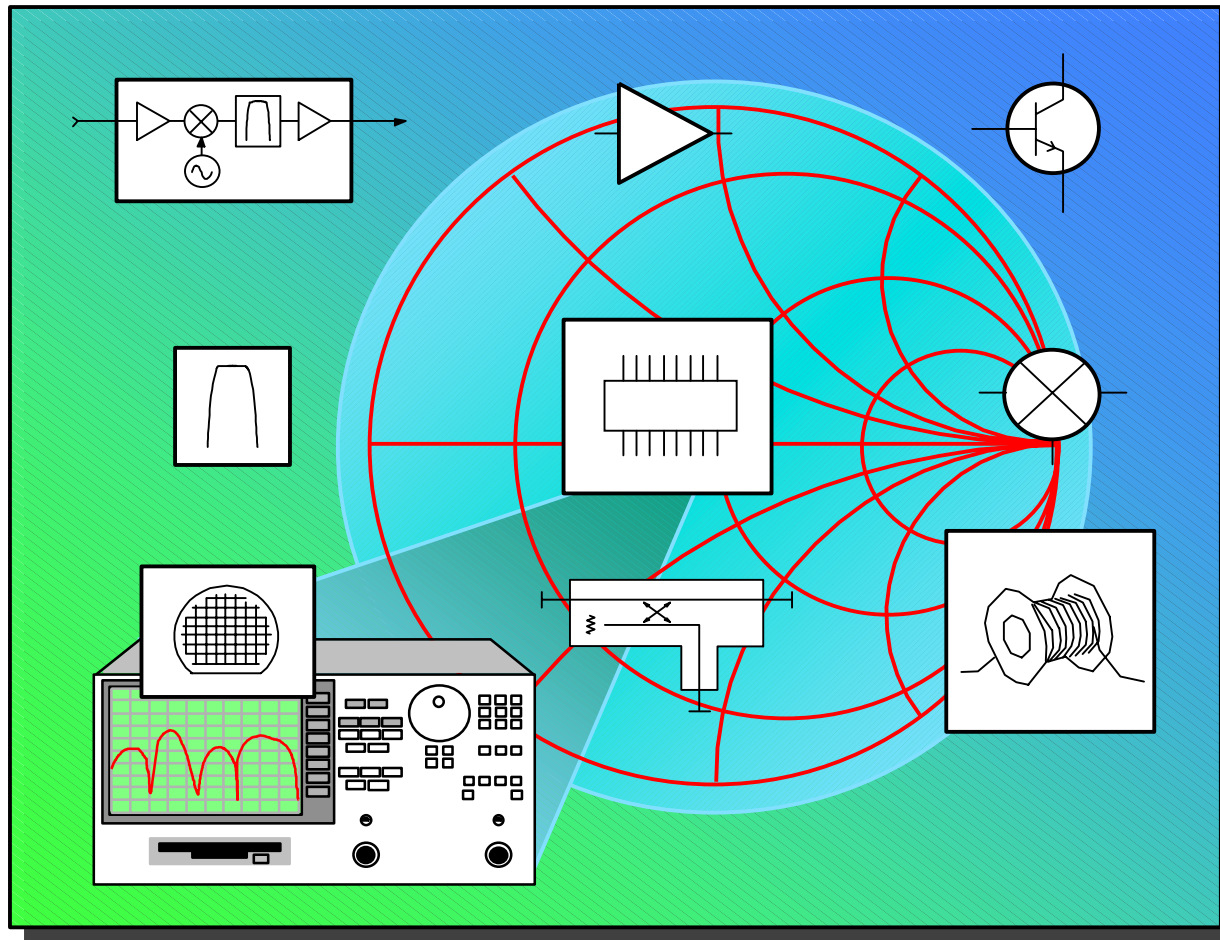


Network Analysis is NOT. ...

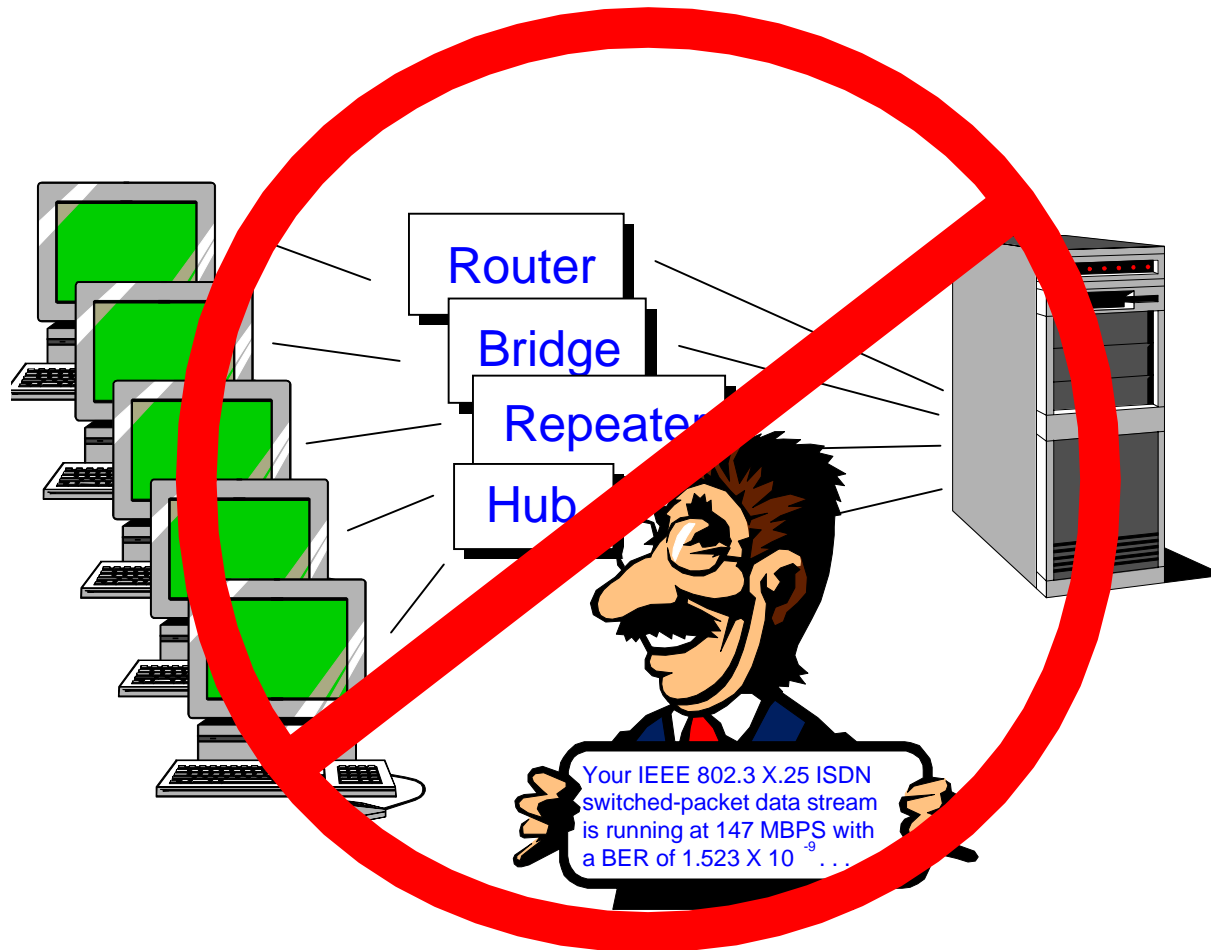



What Types of Devices are Tested?

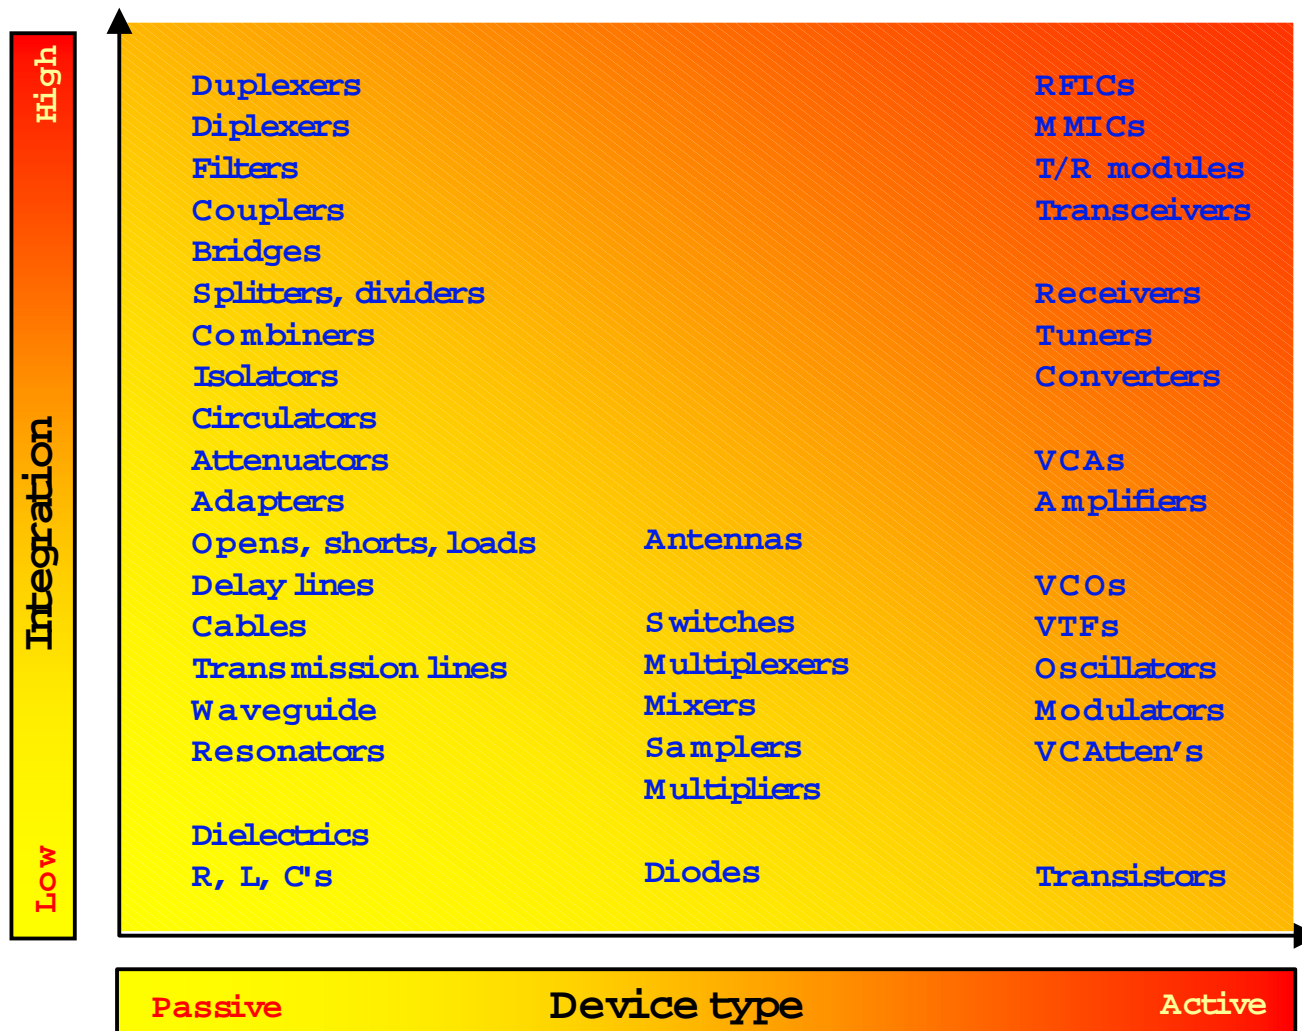

Device Test Measurement Model

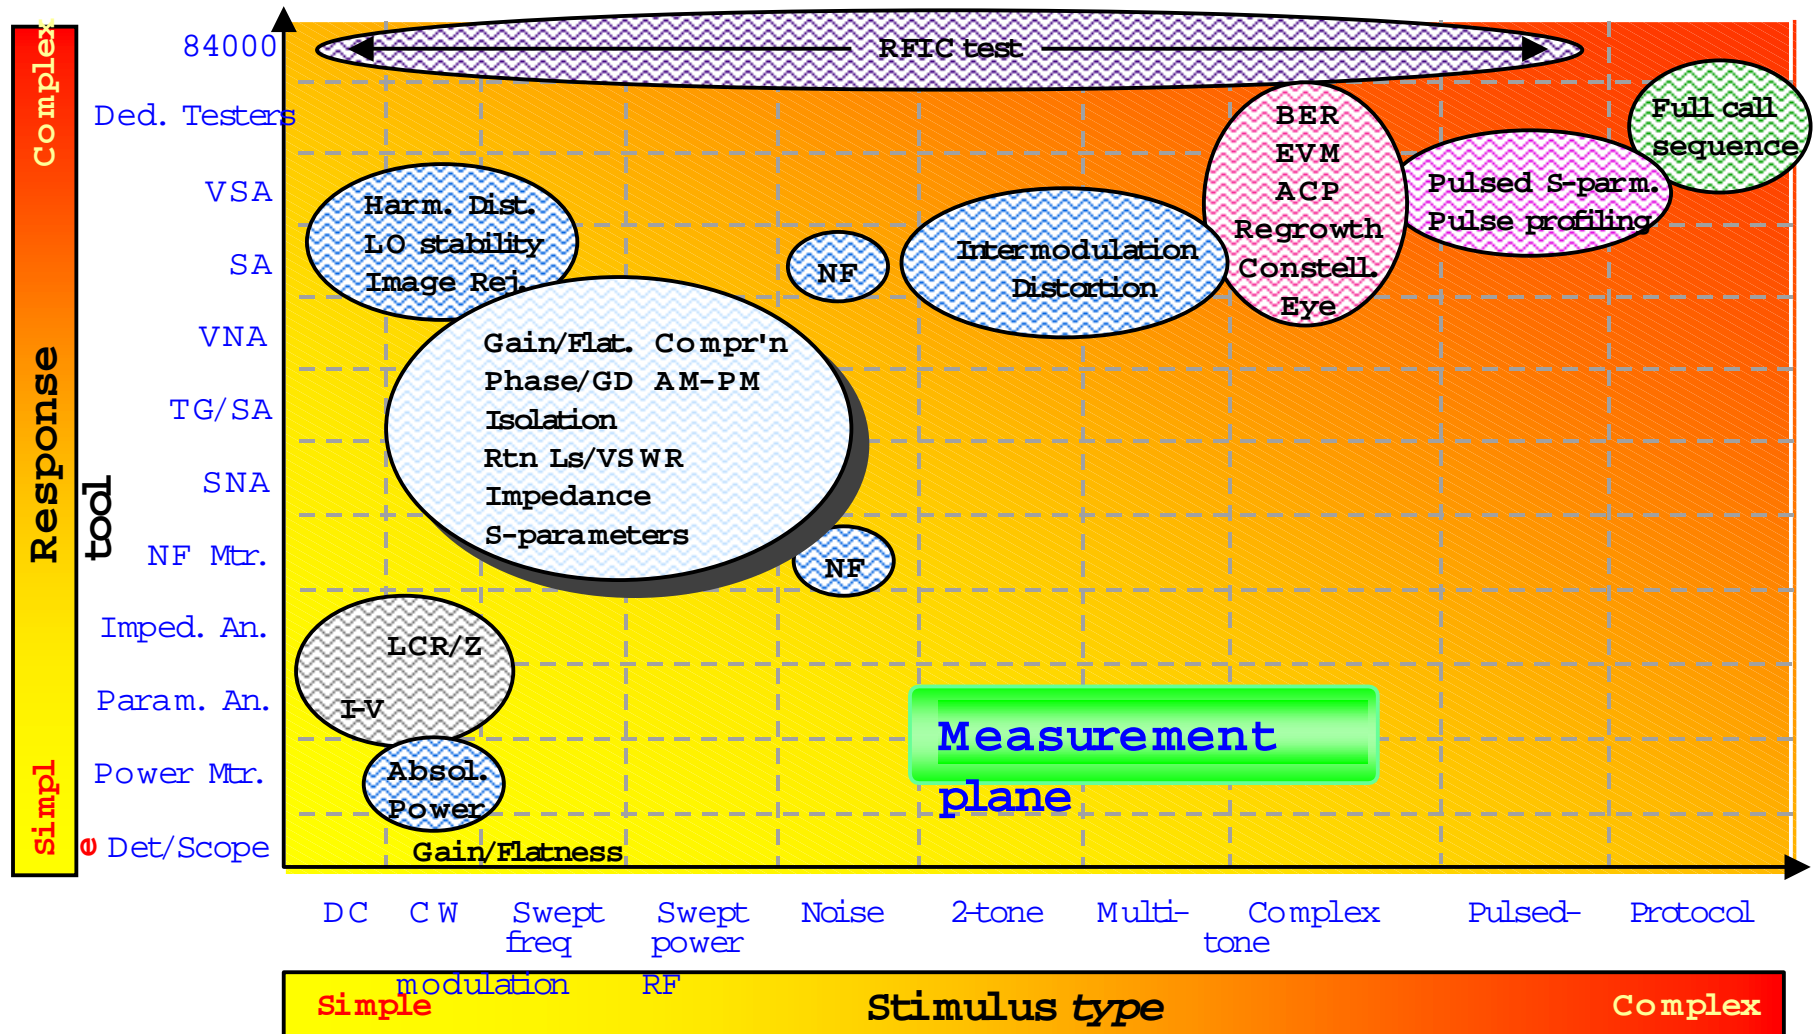


Lightwave Analogy to RF Energy

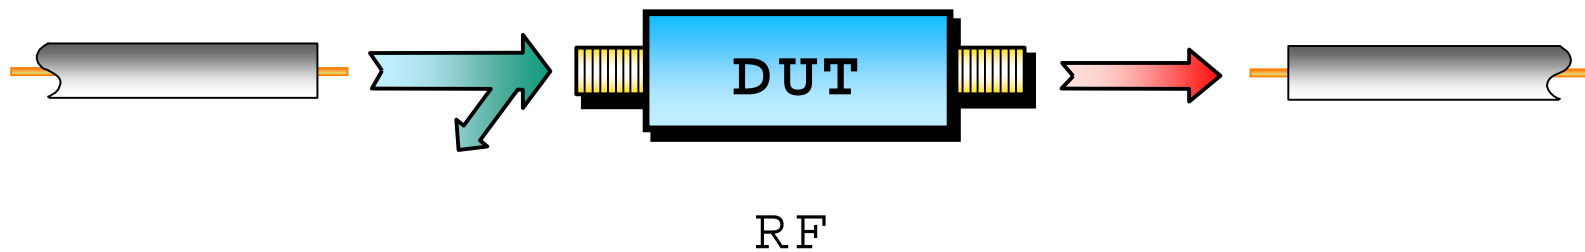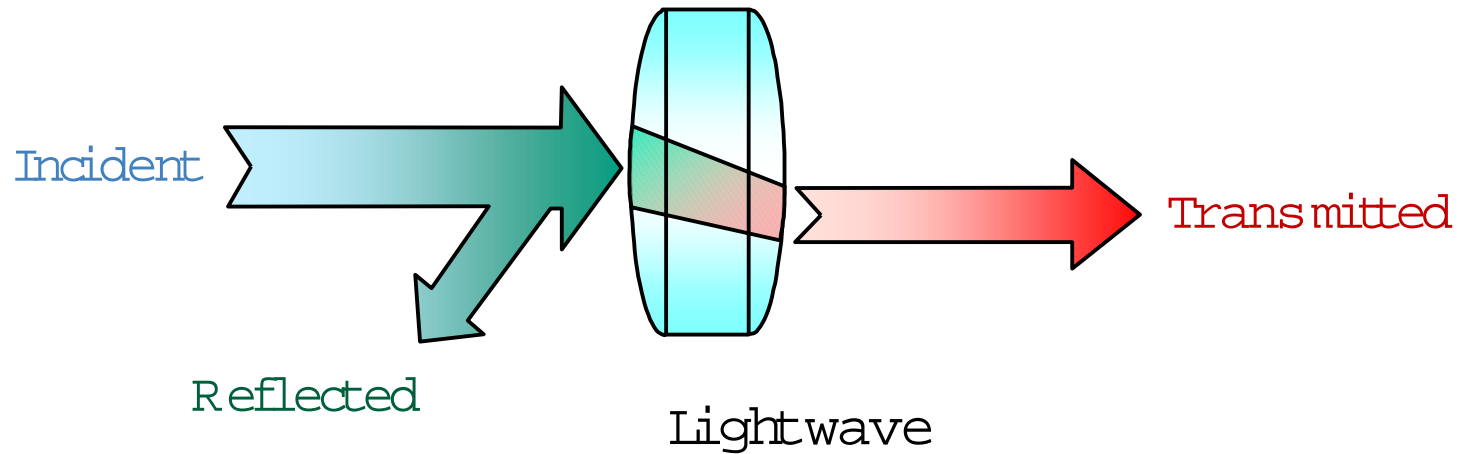


Why Do We Need to Test Components?

- Verify specifications of "building blocks" for more complex RF systems
- Ensure distortionless transmission of communications signals
 - linear: constant amplitude, linear phase / constant group delay
 - nonlinear: harmonics, intermodulation, compression, AM-to-PM conversion
- Ensure good match when absorbing power (e.g., an antenna)

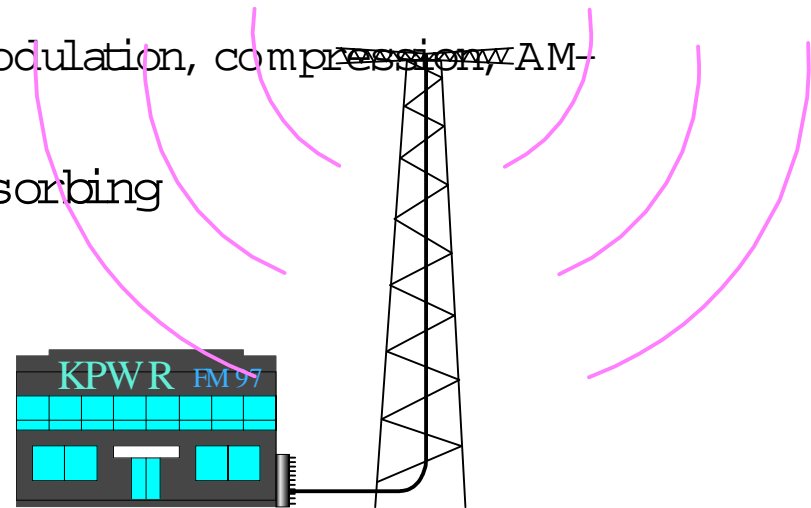


The Need for Both Magnitude and Phase


1. Complete characterization of linear networks

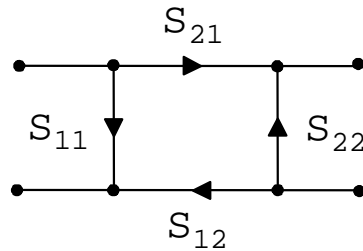


2. Complex impedance needed to design matching circuits




3. Complex values needed for device modeling

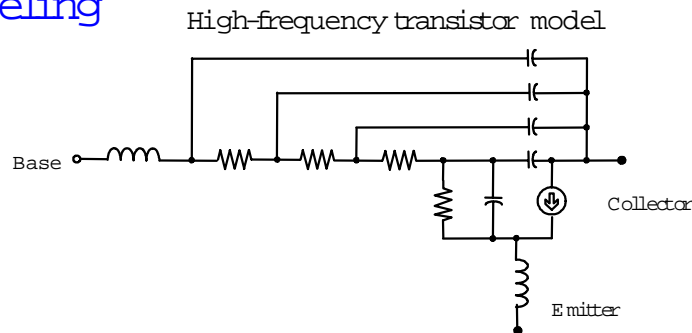


4. Time-domain characterization

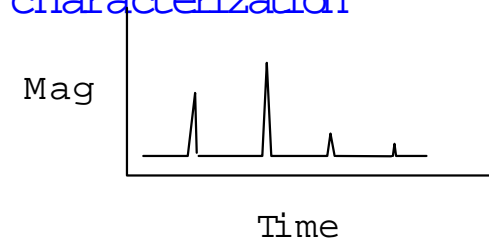

5. Vector-error correction

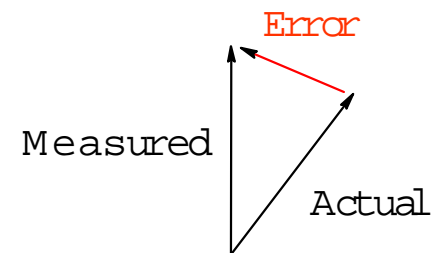

Agenda

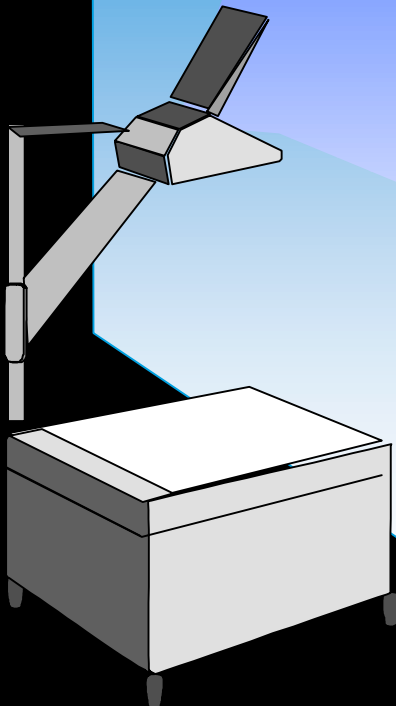


A stylized illustration of a network analyzer setup. It features a white, box-like base unit on wheels. A vertical arm extends from the top of the unit, supporting a horizontal probe arm. The probe arm has a small, dark, rectangular probe head at its end. The background is a dark blue gradient with a lighter blue triangular shape behind the probe arm.

- **What measurements do we make?**
 - Transmission-line basics
 - Reflection and transmission parameters
 - S-parameter definition
- **Network analyzer hardware**
 - Signal separation devices
 - Detection types
 - Dynamic range
 - T/R versus S-parameter test sets
- **Error models and calibration**
 - Types of measurement error
 - One- and two-port models
 - Error-correction choices
 - Basic uncertainty calculations
- **Example measurements**
- **Appendix**




Transmission Line Basics



Low frequencies

- wavelengths \gg wire length
- current (I) travels down wires easily for efficient power transmission
- measured voltage and current not dependent on position along wire

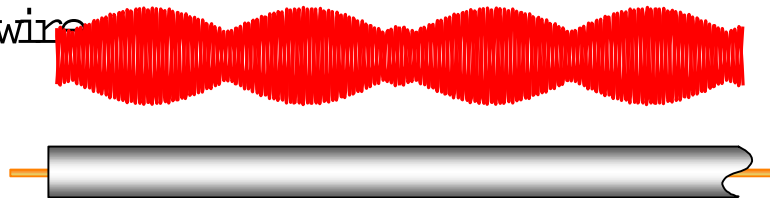



High frequencies

- wavelength \approx or \ll length of transmission medium
- need transmission lines for efficient power transmission
- matching to characteristic impedance (Z_0) is very important for low reflection and maximum power transfer




Transmission line Z_0



- Z_0 determines relationship between voltage and current waves
- Z_0 is a function of physical dimensions and ϵ_r
- Z_0 is usually a real impedance (e.g. 50 or 75 ohms)

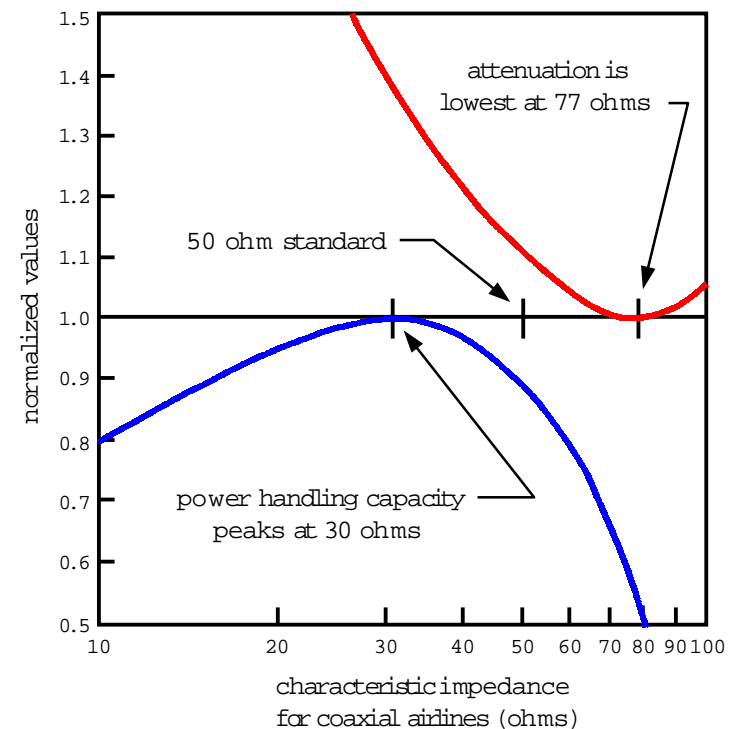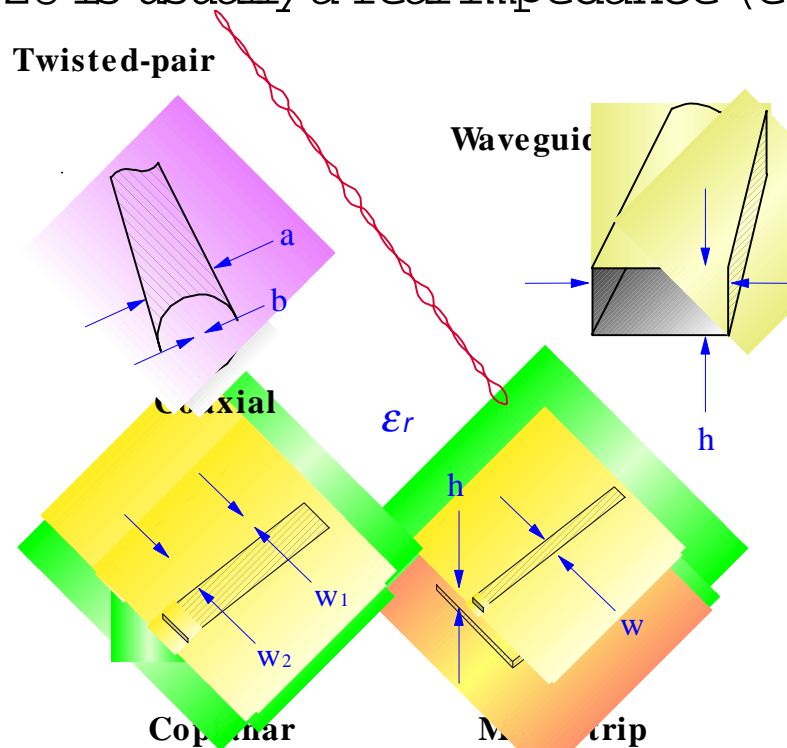

Power Transfer Efficiency

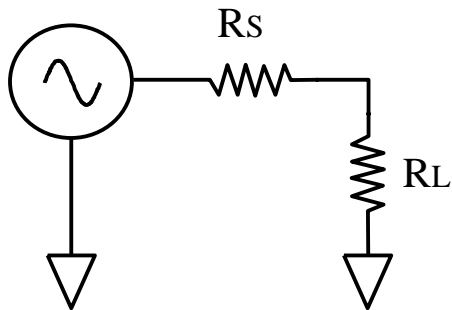


For complex impedances, maximum power transfer occurs when $Z_L = Z_S^*$ (conjugate match)

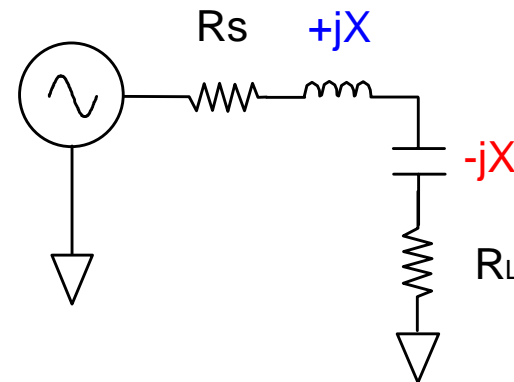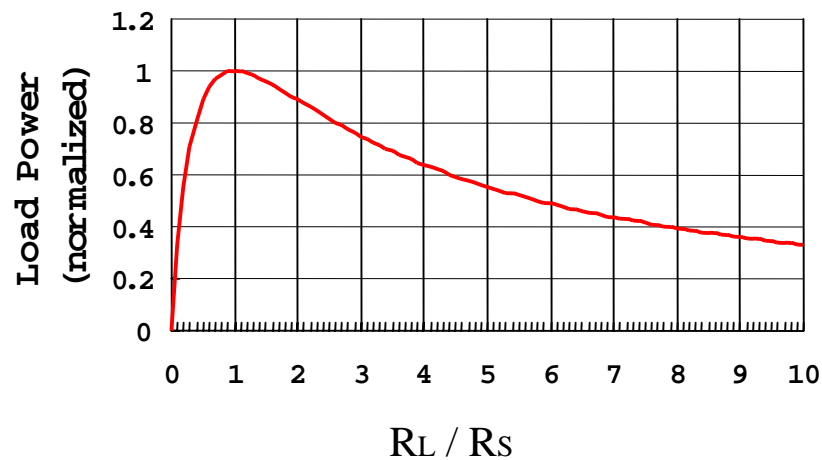

Maximum power is transferred when $R_L = R_S$




Transmission Line Terminated with Z_0

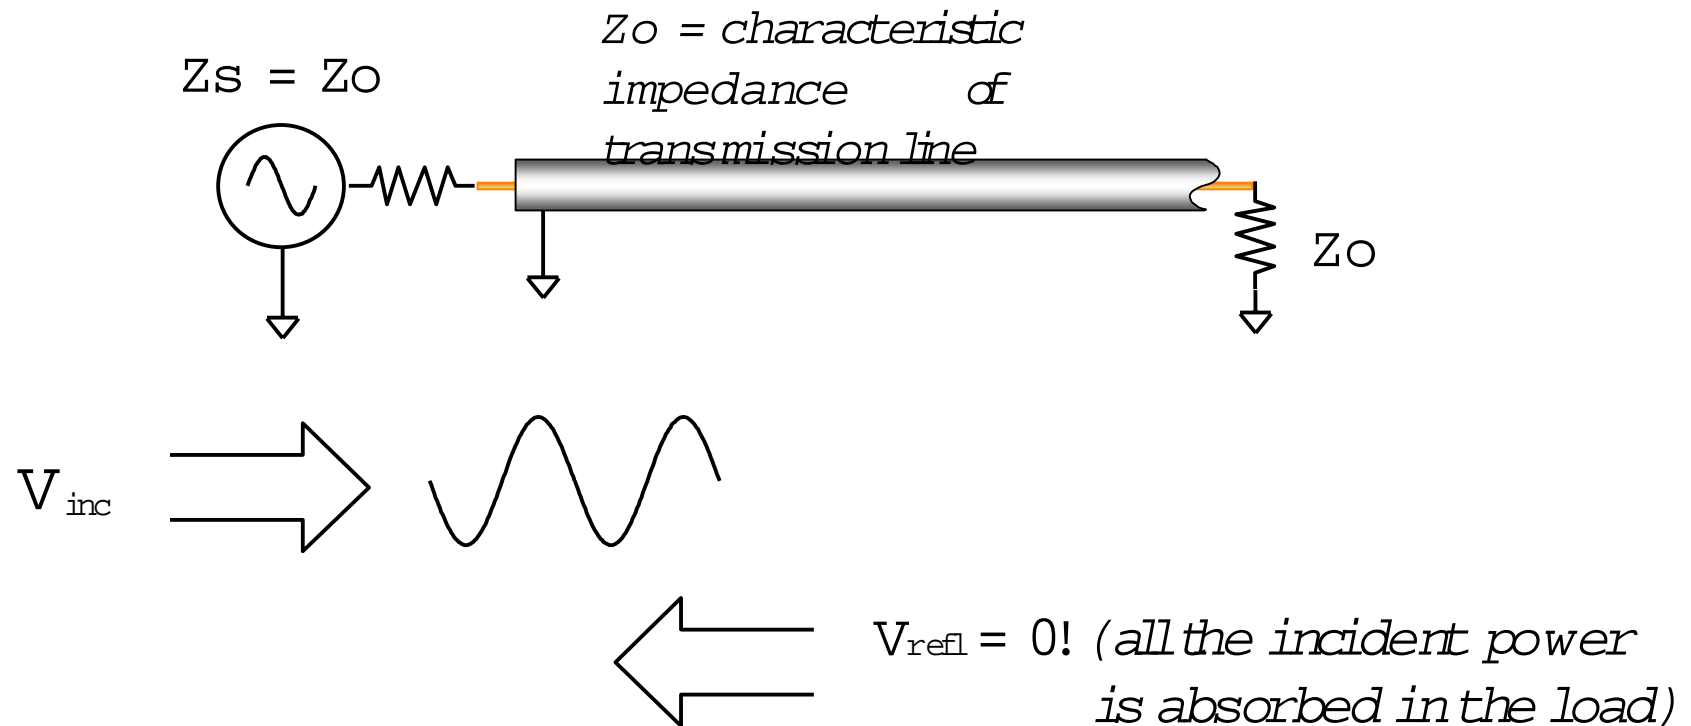

For reflection, a transmission line terminated in Z_0 behaves like an infinitely long transmission line




Transmission Line Terminated with Short, Open

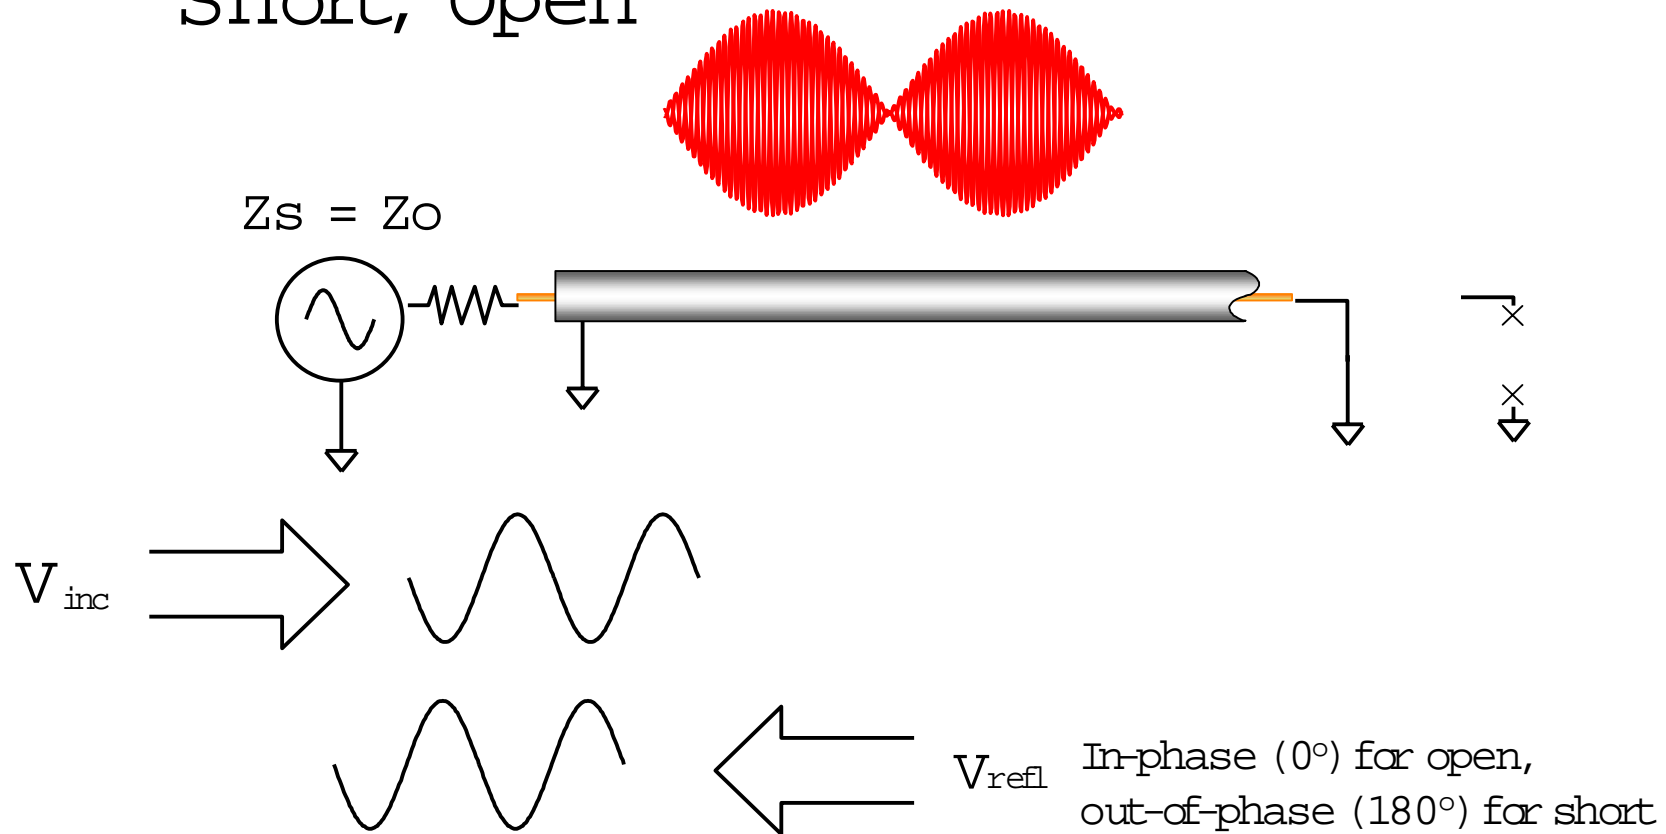


For reflection, a transmission line terminated in a short or open reflects all power back to source

Transmission Line Terminated with $25\ \Omega$

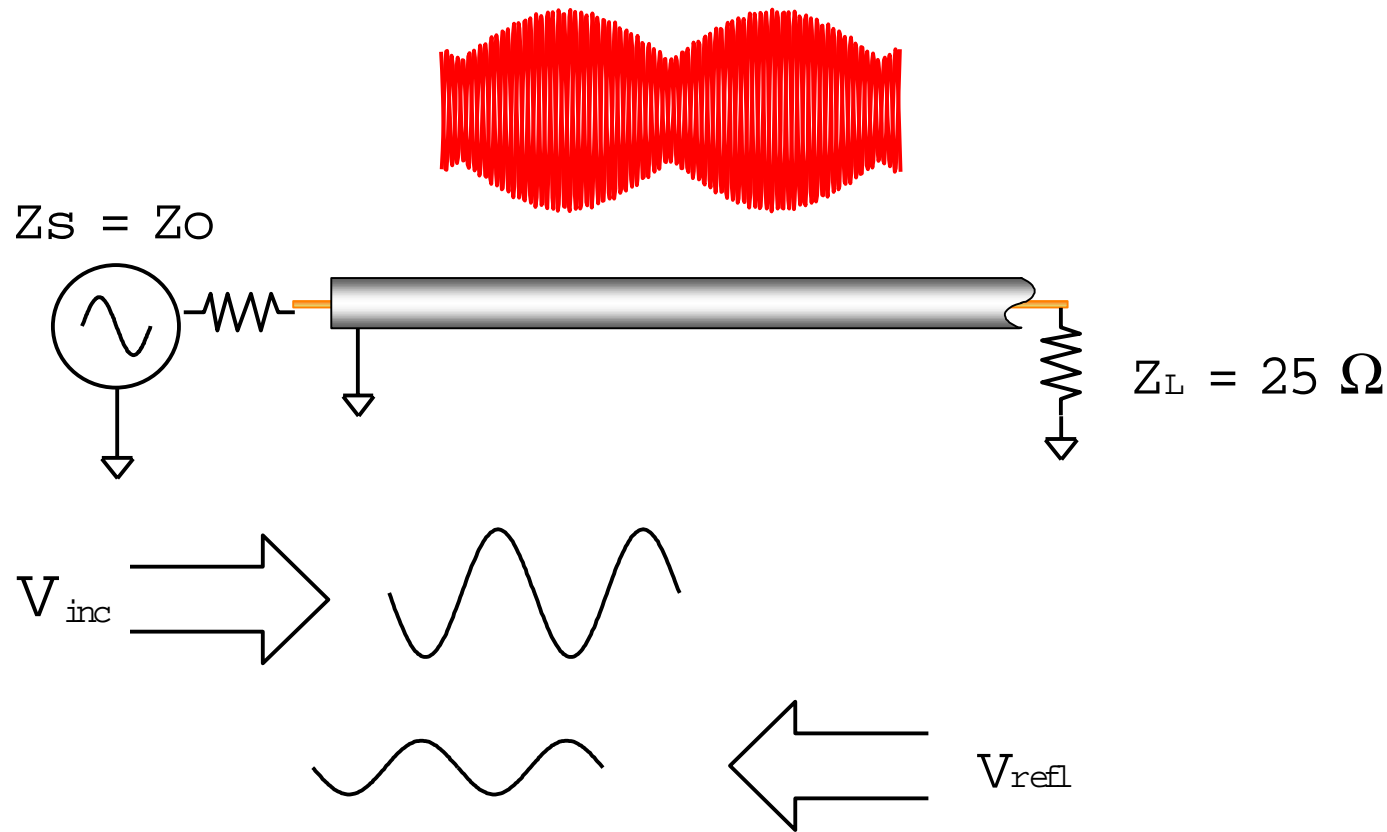


Standing wave pattern
does not go to zero as
with short or open

High-Frequency Device Characterization

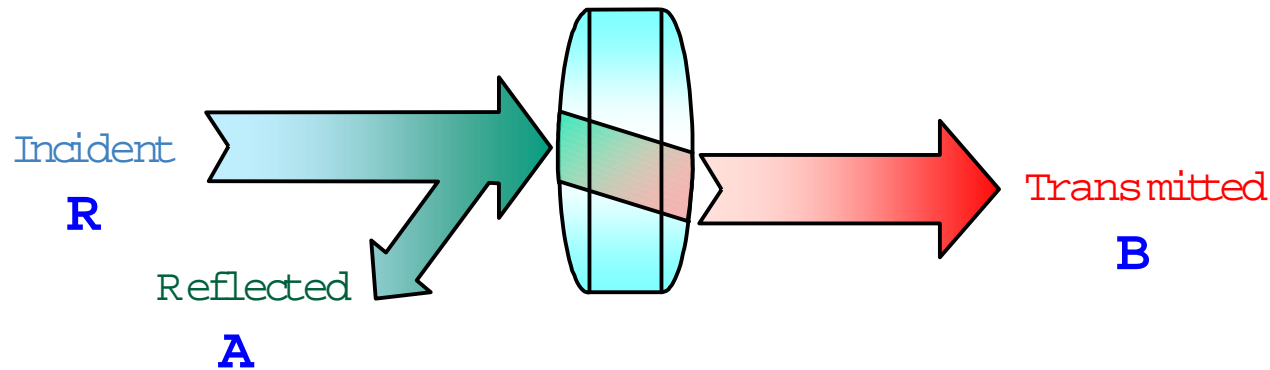


REFLECTION

$$\frac{\text{Reflected}}{\text{Incident}} = \frac{A}{R}$$

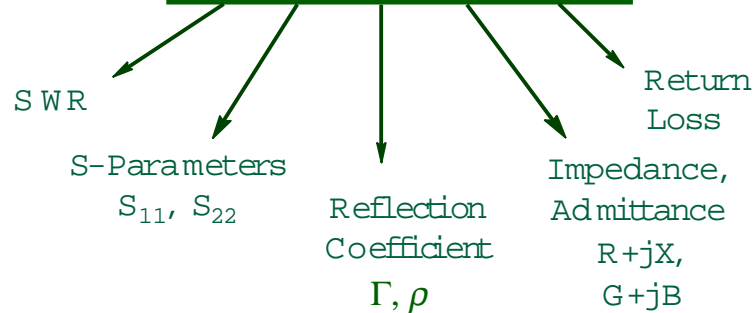

TRANSMISSION


$$\frac{\text{Transmitted}}{\text{Incident}} = \frac{B}{R}$$

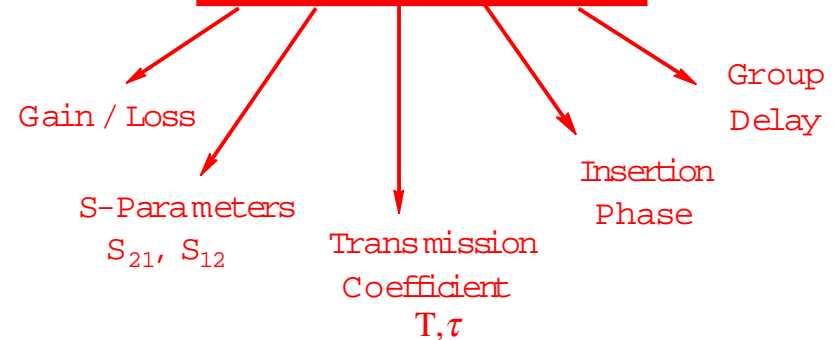

Reflection Parameters

Reflection Coefficient $\Gamma = \frac{V_{\text{reflected}}}{V_{\text{incident}}} = \rho \angle \Phi = \frac{Z_L - Z_0}{Z_L + Z_0}$

Return loss $= -20 \log(\rho), \rho = |\Gamma|$

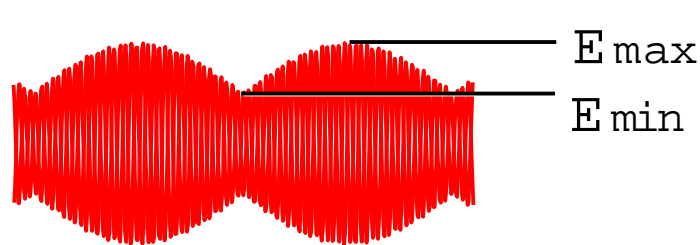

Voltage Standing Wave Ratio

VSWR $= \frac{E_{\text{max}}}{E_{\text{min}}} = \frac{1 + \rho}{1 - \rho}$


No reflection
($Z_L = Z_0$)

Full reflection
($Z_L = \text{open, short}$)


0	ρ	1
∞ dB	RL	0 dB
1	VSWR	∞



Smith Chart Review

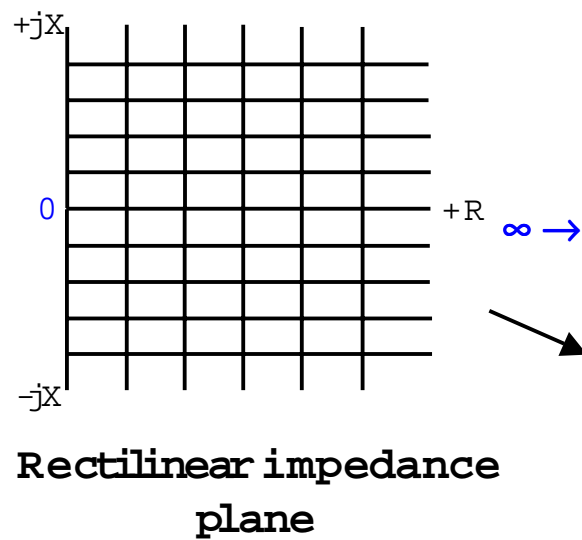

Smith Chart maps
rectilinear
impedance
plane onto polar
plane

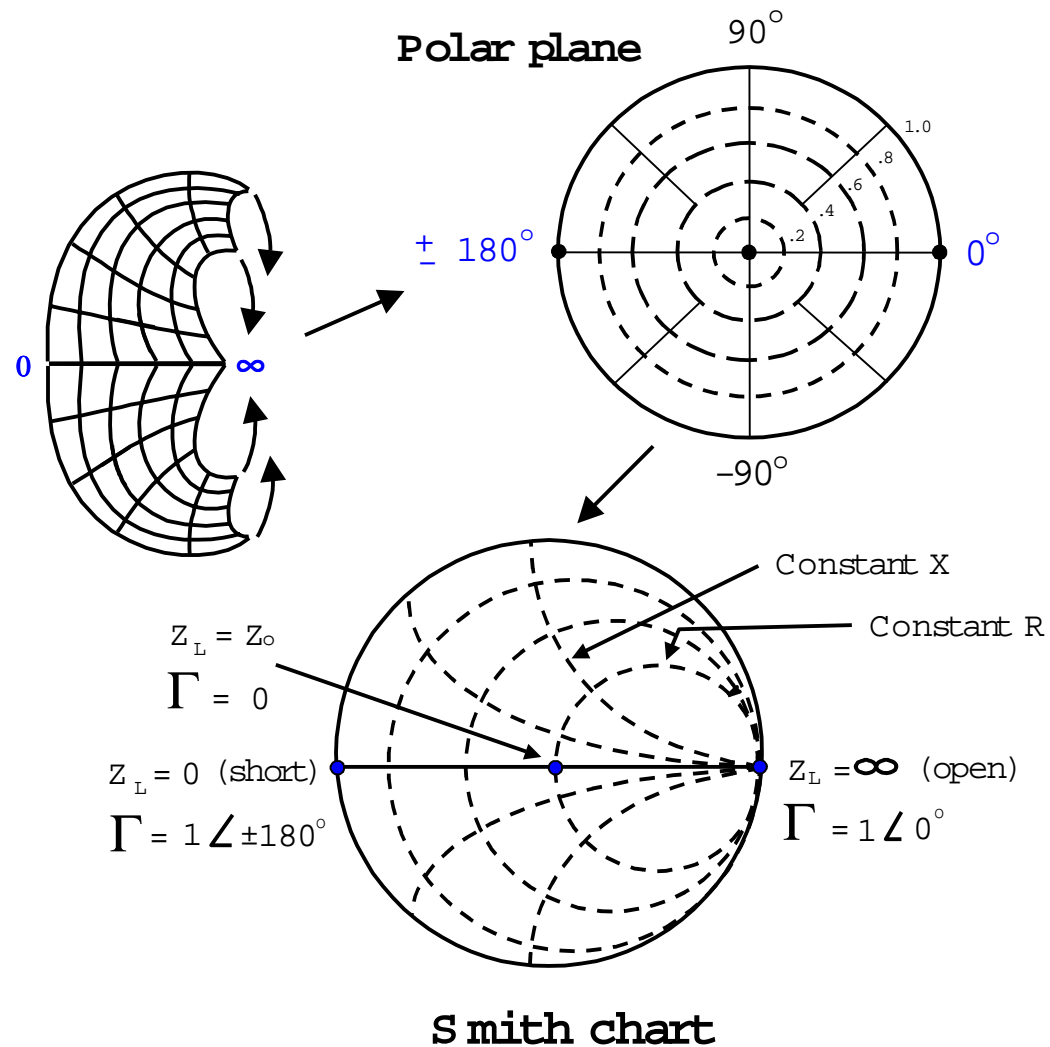

Transmission Parameters




$$\text{Transmission Coefficient} = T = \frac{V_{\text{Transmitted}}}{V_{\text{Incident}}} = \tau \angle \phi$$

$$\text{Insertion Loss (dB)} = -20 \log \left| \frac{V_{\text{Trans}}}{V_{\text{Inc}}} \right| = -20 \log \tau$$

$$\text{Gain (dB)} = 20 \log \left| \frac{V_{\text{Trans}}}{V_{\text{Inc}}} \right| = 20 \log \tau$$





Linear Versus Nonlinear Behavior

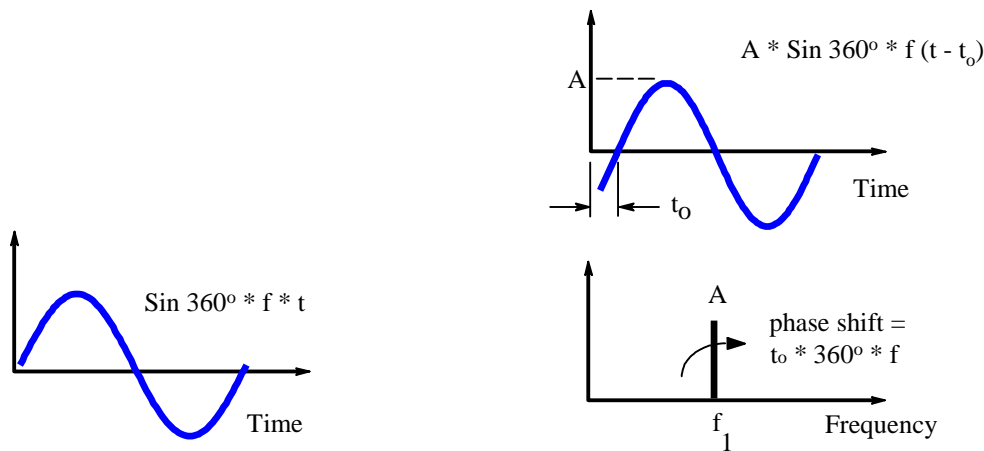

Linear behavior:

- input and output frequencies are the same (no additional frequencies created)
- output frequency only undergoes magnitude and phase change

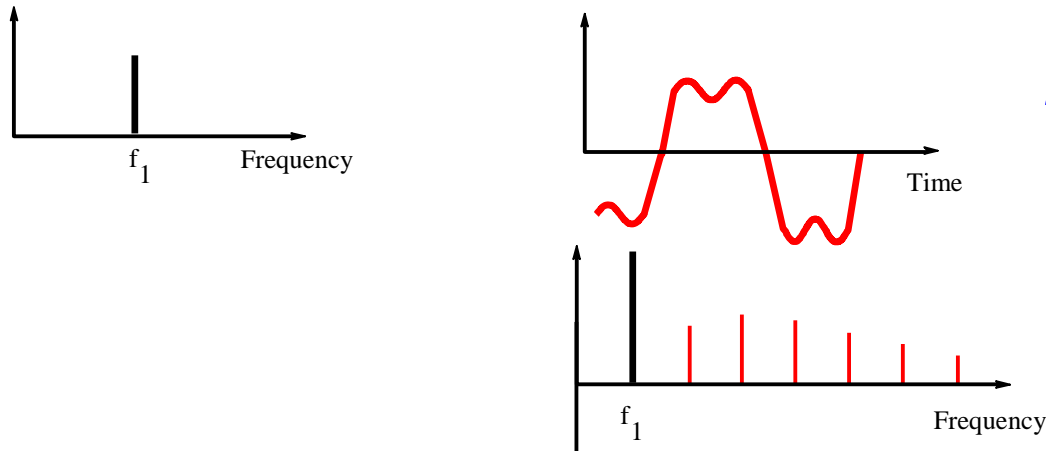


Nonlinear behavior:

- output frequency may undergo frequency shift (e.g. with mixers)
- additional frequencies created (harmonics, intermodulation)




Criteria for Distortionless Transmission

Linear Networks

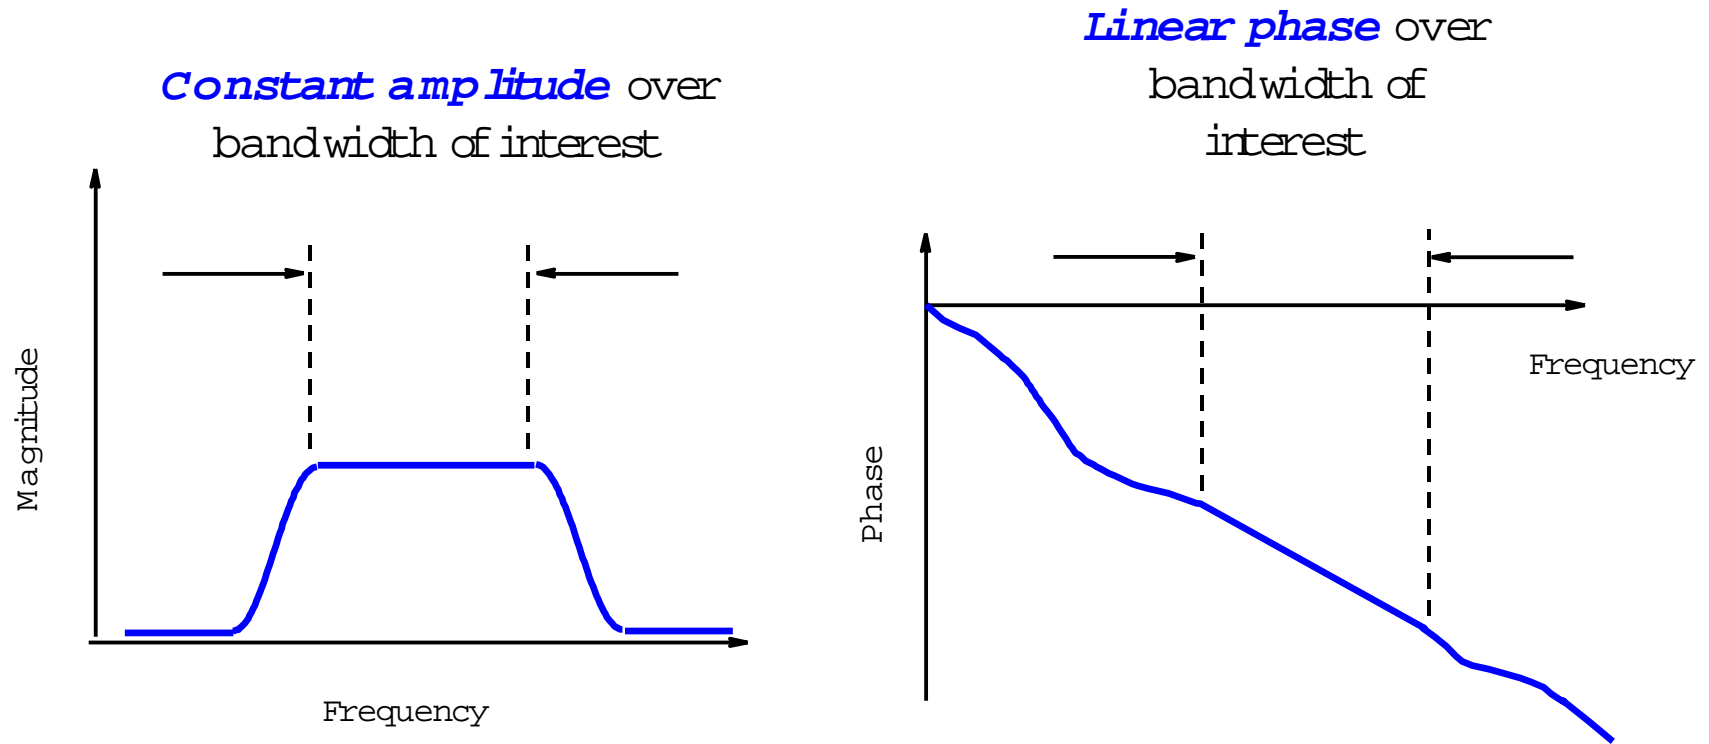


Magnitude Variation with Frequency

$$F(t) = \sin \omega t + \frac{1}{3} \sin 3\omega t + \frac{1}{5} \sin 5\omega t$$

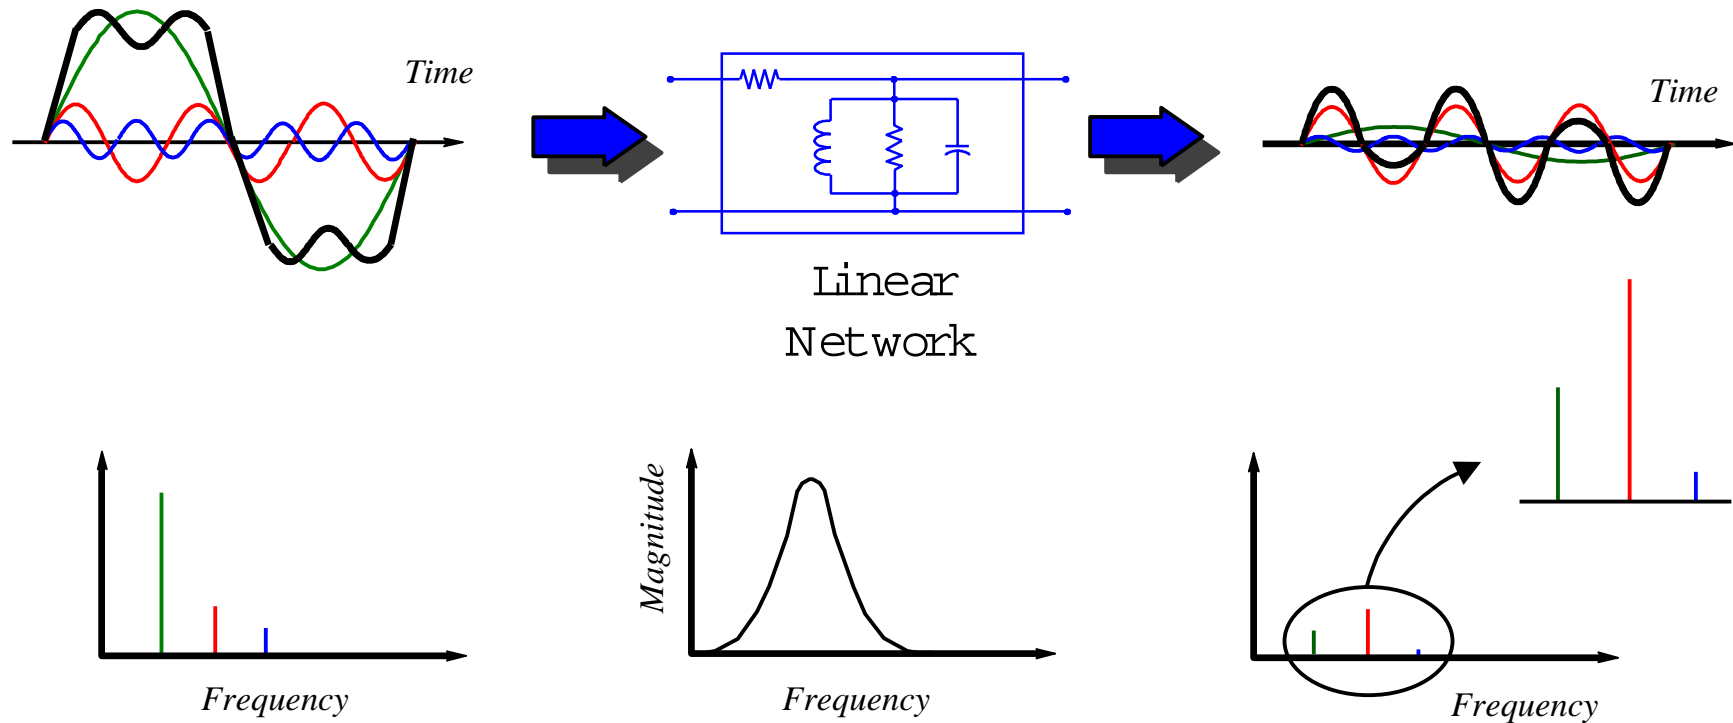


Phase Variation with Frequency

$$F(t) = \sin \omega t + \frac{1}{3} \sin 3\omega t + \frac{1}{5} \sin 5\omega t$$


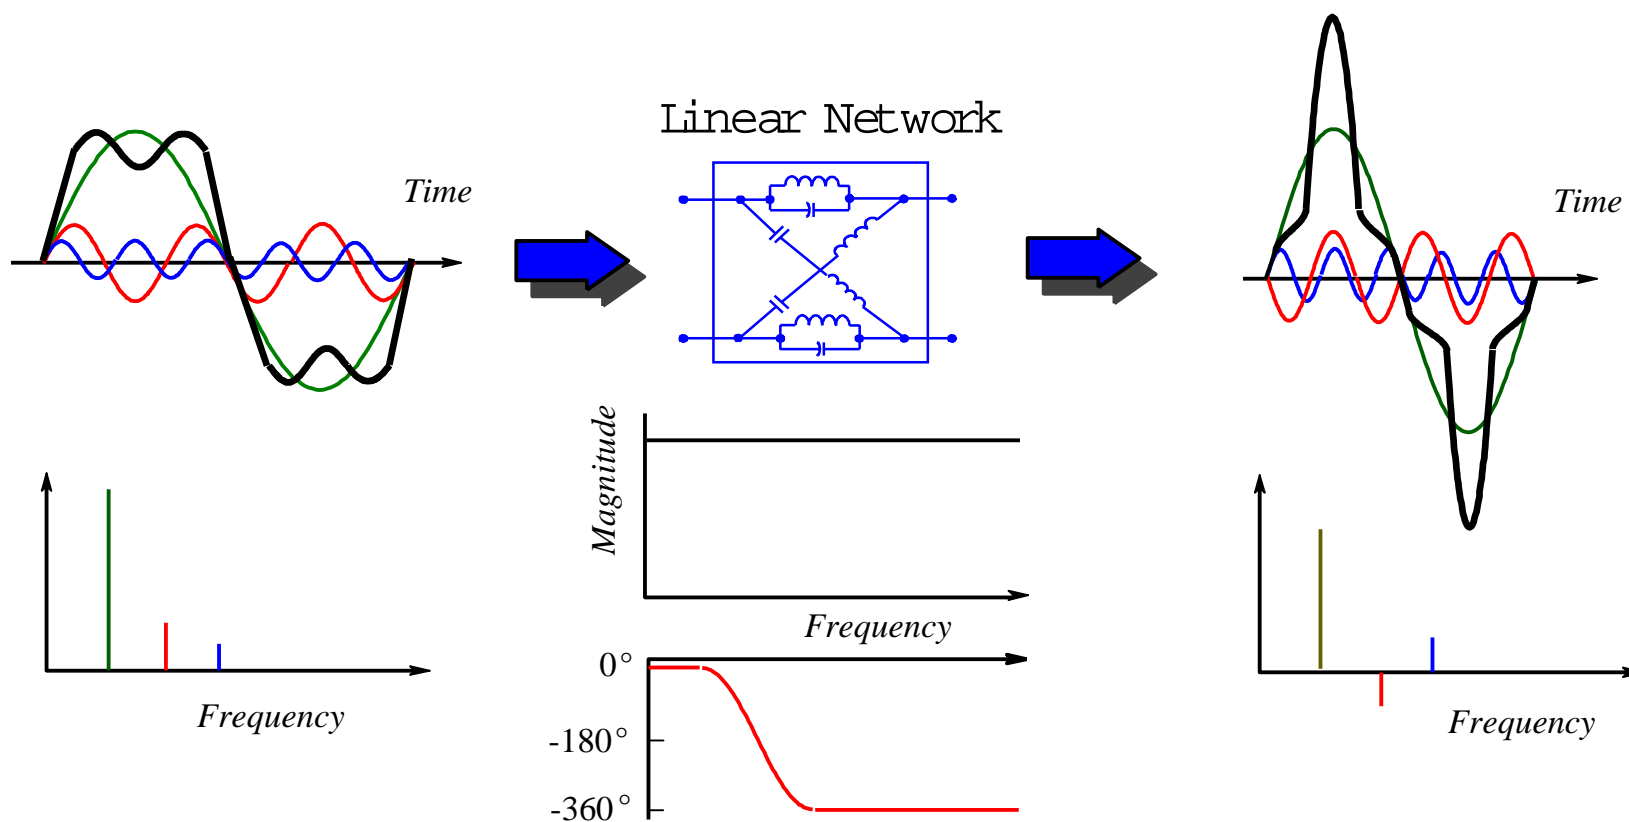


Deviation from Linear Phase

*Use electrical delay to
remove linear portion of
phase response*

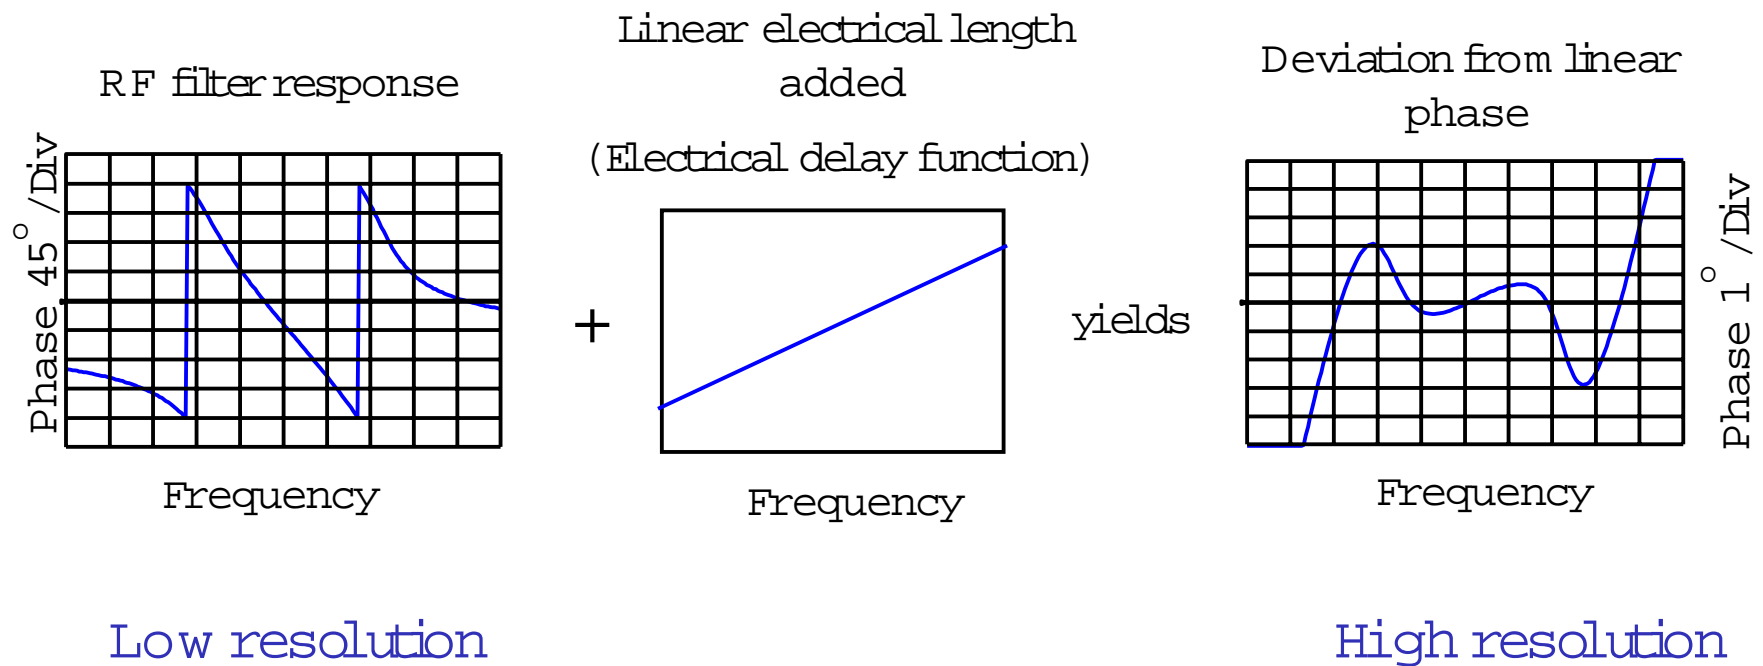

Group Delay

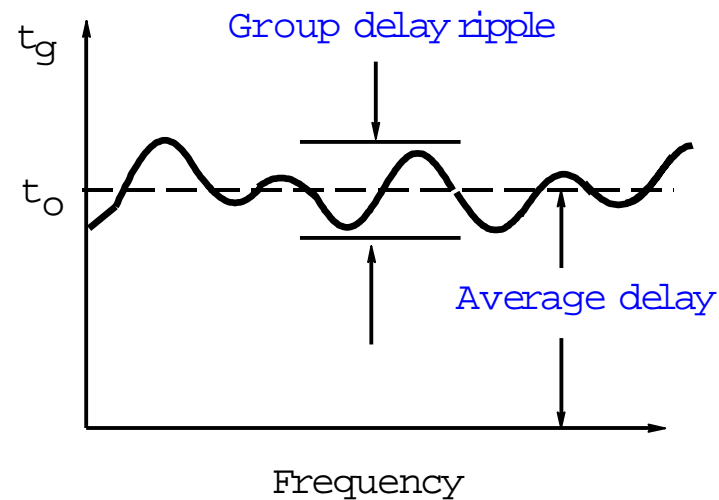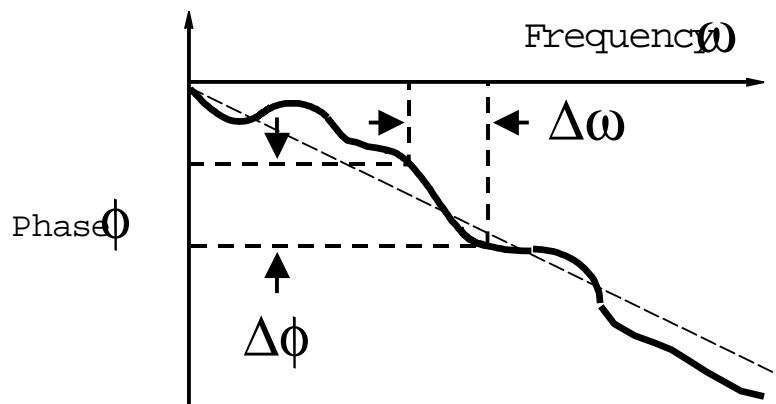

Group Delay (t_g) =

$$\frac{-d\phi}{d\omega} = \frac{-1}{360^\circ} * \frac{d\phi}{df}$$

ϕ in radians

ω in radians/sec


ϕ in degrees

f in Hertz ($\omega = 2\pi f$)

- group-delay ripple indicates phase distortion
- average delay indicates electrical length of DUT
- aperture of measurement is very important



Why Measure Group Delay?

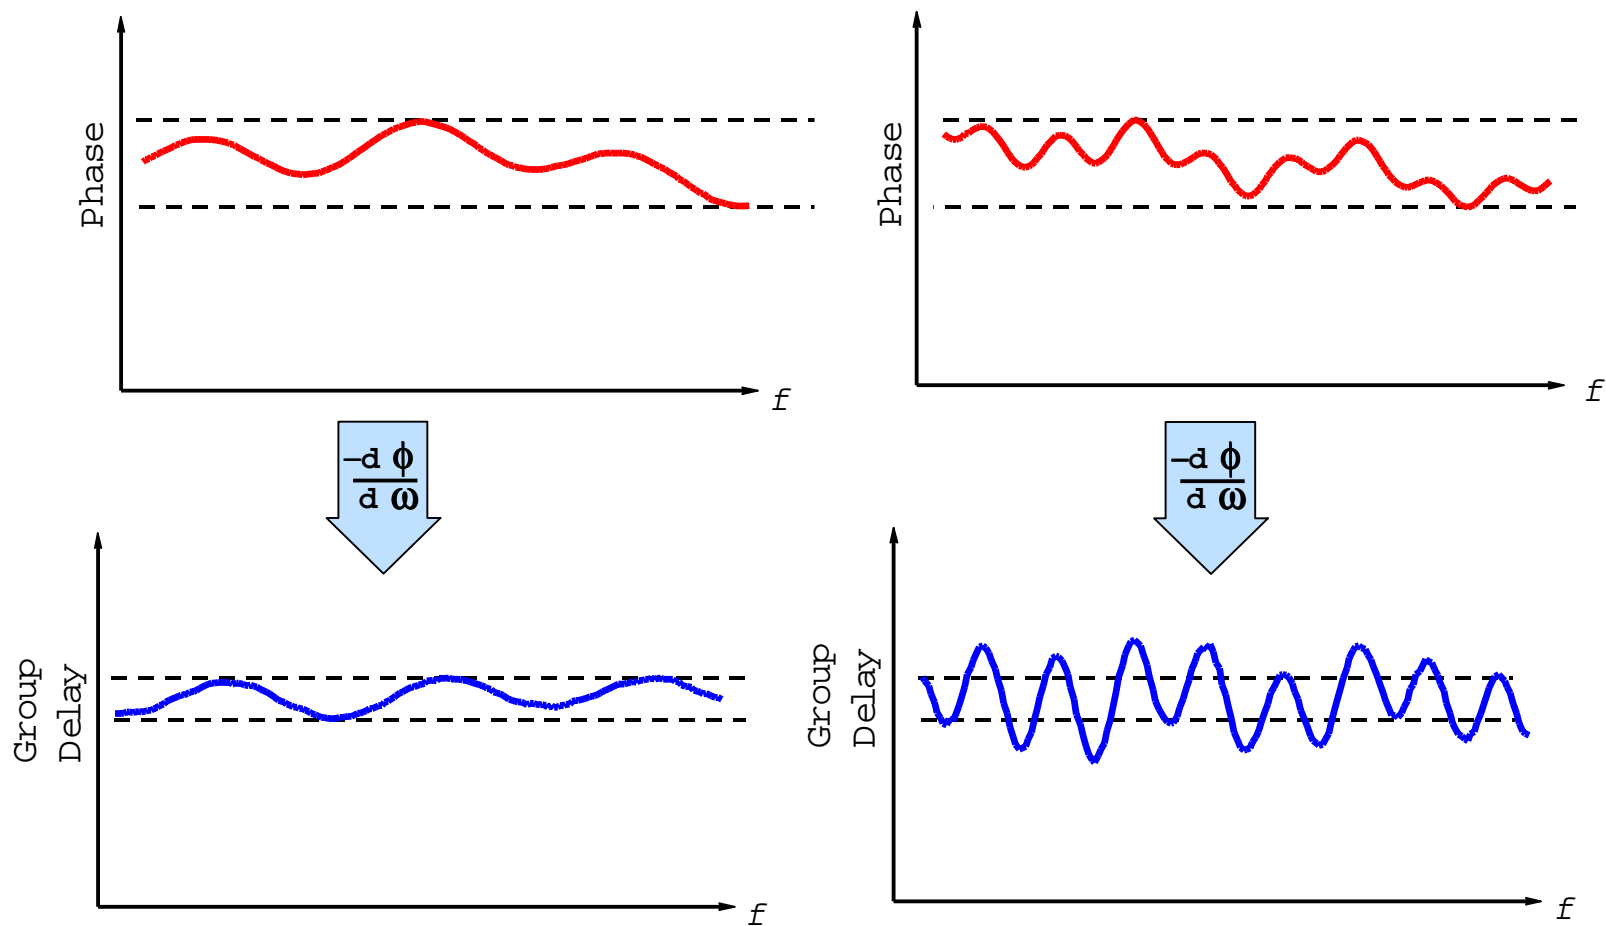

Same p-p phase ripple can result in different
group delay



Characterizing Unknown Devices

Using parameters (H, Y, Z, S) to characterize devices:

- gives linear behavioral model of our device
- measure parameters (e.g. voltage and current) versus frequency under various source and load conditions (e.g. short and open circuits)
- compute device parameters from measured data
- predict circuit performance under any source and load conditions

H-parameters

$$V_1 = h_{11}I_1 + h_{12}V_2$$

$$I_2 = h_{21}I_1 + h_{22}V_2$$

Y-parameters


$$I_1 = y_{11}V_1 + y_{12}V_2$$

$$I_2 = y_{21}V_1 + y_{22}V_2$$

Z-parameters

$$V_1 = z_{11}I_1 + z_{12}I_2$$

$$V_2 = z_{21}I_1 + z_{22}I_2$$





$$h_{11} = \left. \frac{V_1}{I_1} \right|_{V_2=0} \quad (\text{requires } \textbf{short circuit})$$

$$h_{12} = \left. \frac{V_1}{V_2} \right|_{I_1=0} \quad (\text{requires } \textbf{open circuit})$$



Why Use S-Parameters?

- relatively easy to **obtain** at high frequencies
 - measure voltage traveling waves with a vector network analyzer
 - don't need shorts/opens which can cause active devices to oscillate or self-destruct
- relate to **familiar** measurements (gain, loss, reflection coefficient ...)
- can **cascade** S-parameters of multiple devices to predict system performance
- can **compute** H, Y, or Z parameters from S-parameters if desired
- can easily import and use S-parameter files in our **electronic-simulation** tools

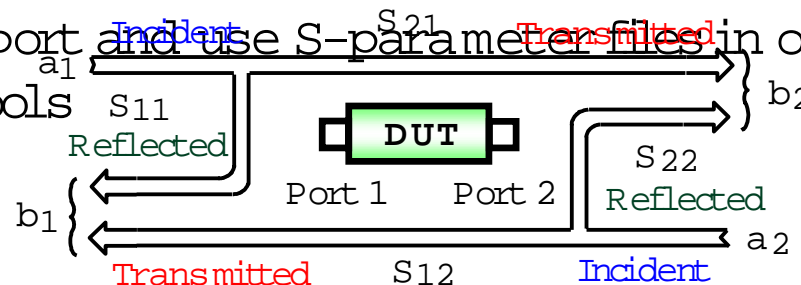


$$b_1 = S_{11}a_1 + S_{12}a_2$$

$$b_2 = S_{21}a_1 + S_{22}a_2$$



Measuring S-Parameters

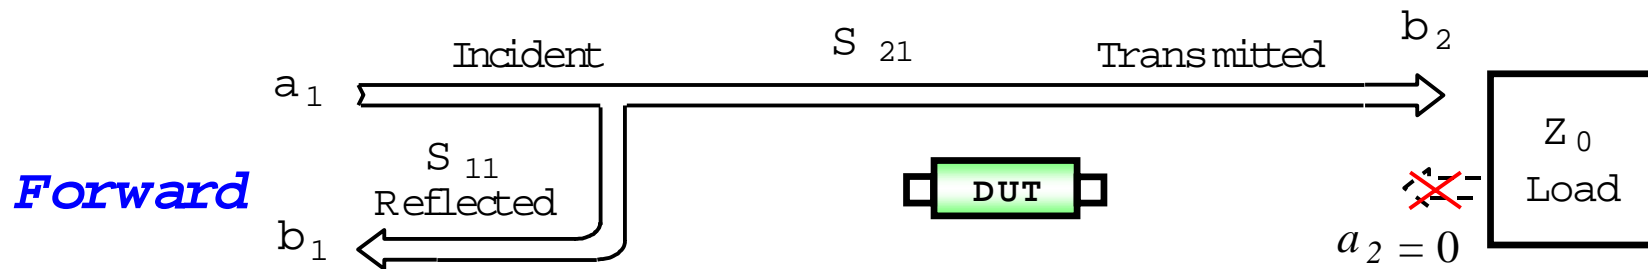


$$S_{11} = \frac{\text{Reflected}}{\text{Incident}} = \frac{b_1}{a_1} \Big|_{a_2 = 0}$$

$$S_{21} = \frac{\text{Transmitted}}{\text{Incident}} = \frac{b_2}{a_1} \Big|_{a_2 = 0}$$

$$S_{22} = \frac{\text{Reflected}}{\text{Incident}} = \frac{b_2}{a_2} \Big|_{a_1 = 0}$$

$$S_{12} = \frac{\text{Transmitted}}{\text{Incident}} = \frac{b_1}{a_2} \Big|_{a_1 = 0}$$

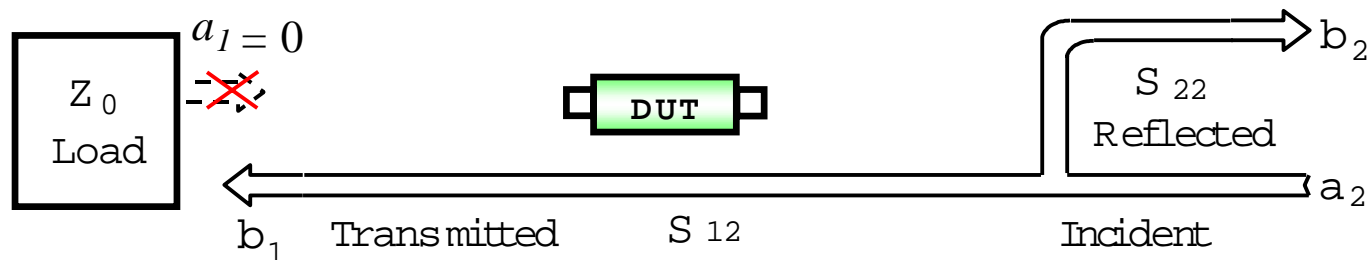

Reverse



Equating S-Parameters with Common Measurement Terms

S_{11} = forward reflection coefficient (*input match*)

S_{22} = reverse reflection coefficient (*output match*)

S_{21} = forward transmission coefficient (*gain or loss*)

S_{12} = reverse transmission coefficient (*isolation*)


Remember, S-parameters are inherently complex, linear quantities — however, we often express them in a log-magnitude format



Criteria for Distortionless Transmission

Nonlinear Networks



- Saturation, crossover, intermodulation, and other nonlinear effects can cause signal distortion
- Effect on system depends on amount and type of distortion and system architecture

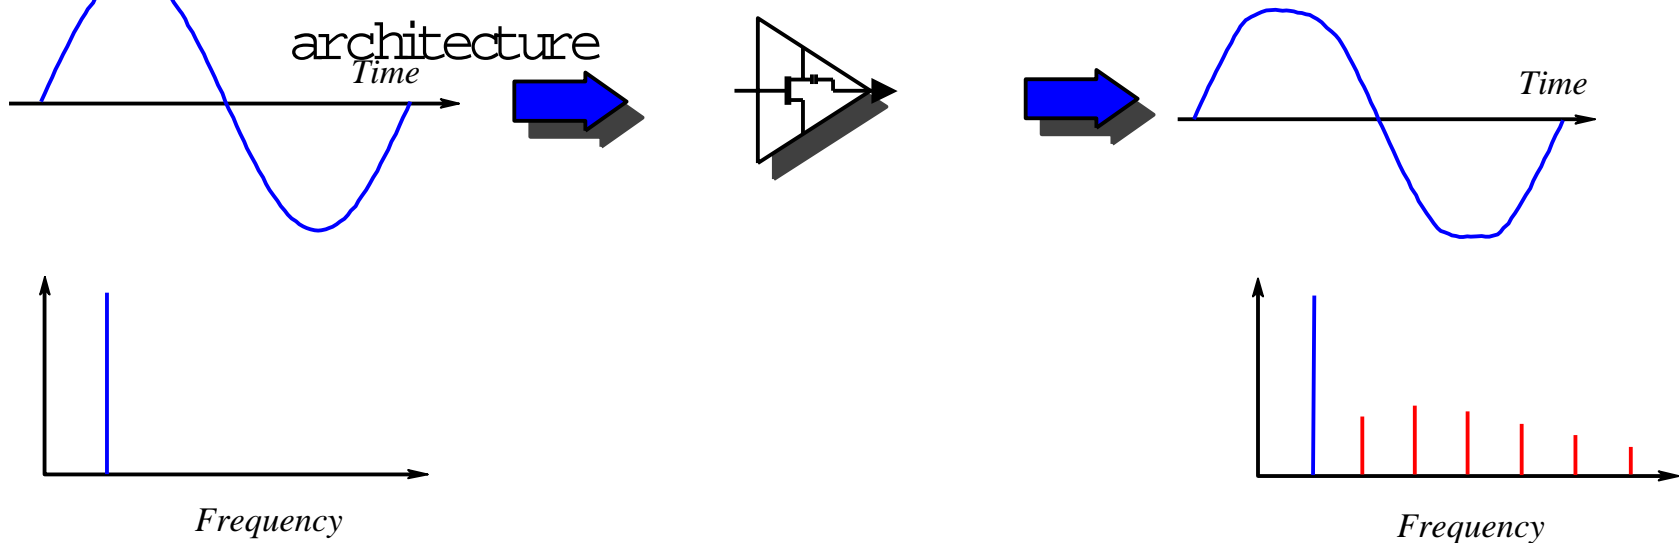



Measuring Nonlinear Behavior

Most common measurements:



- using a **network analyzer** and power sweeps
 - gain compression
 - AM to PM conversion
- using a **spectrum analyzer** + source(s)
 - harmonics, particularly second and third

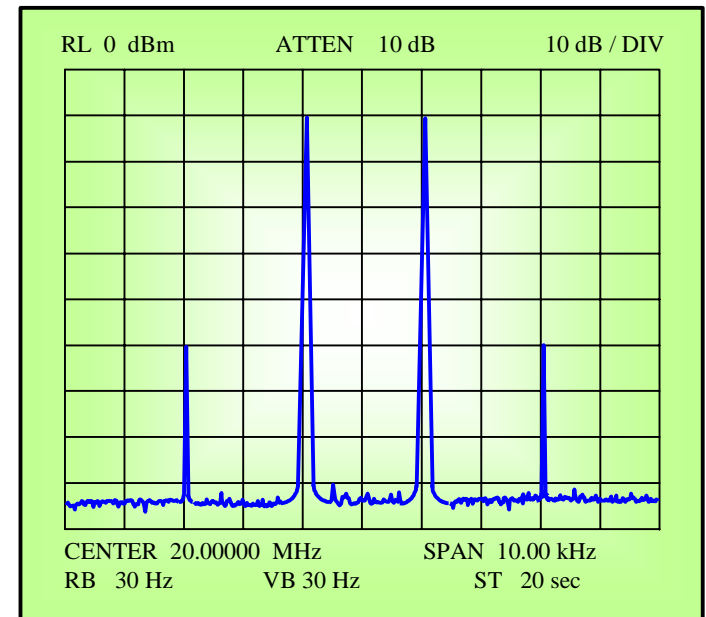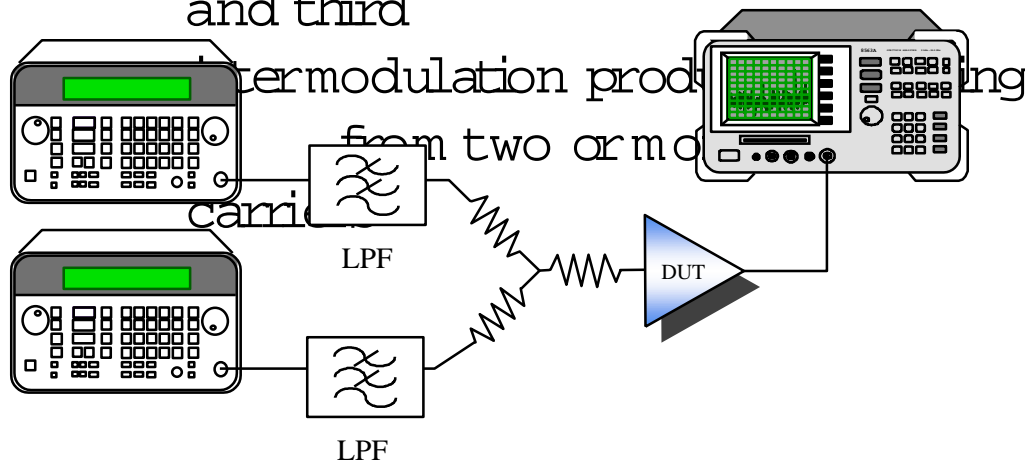

What is the Difference Between **Network** and **Spectrum** Analyzers?

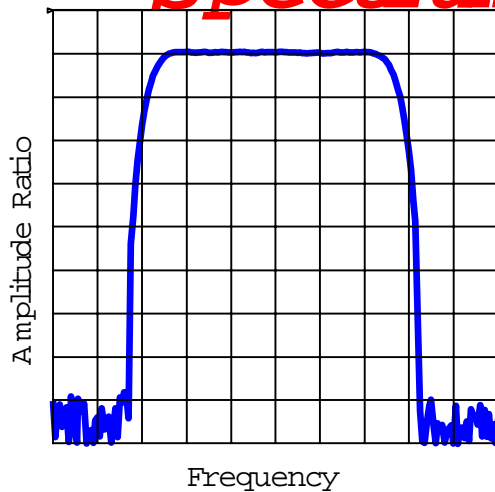

Measures
known
signal

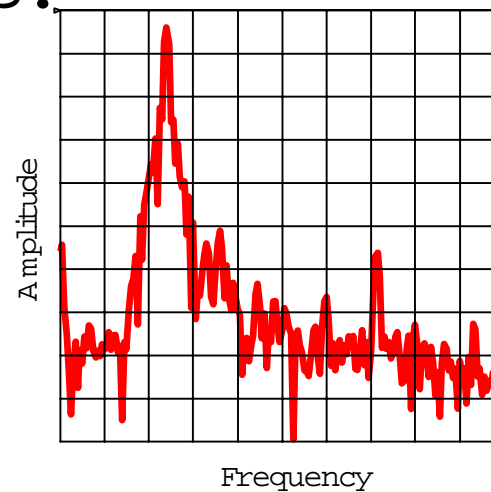

Measures
unknown
signals

Network analyzers:

- measure components, devices, circuits, sub-assemblies
- contain source and receiver
- display ratioed amplitude and phase

(frequency or power sweeps)

- offer advanced error correction

Network Analyzer Basics



Agilent Technologies


Spectrum analyzers:

- measure signal amplitude characteristics (carrier level, sidebands, harmonics...)
- can demodulate (& measure) complex signals
- are receivers only (single channel)

can be used for scalar component test (no


© 2000

Agenda

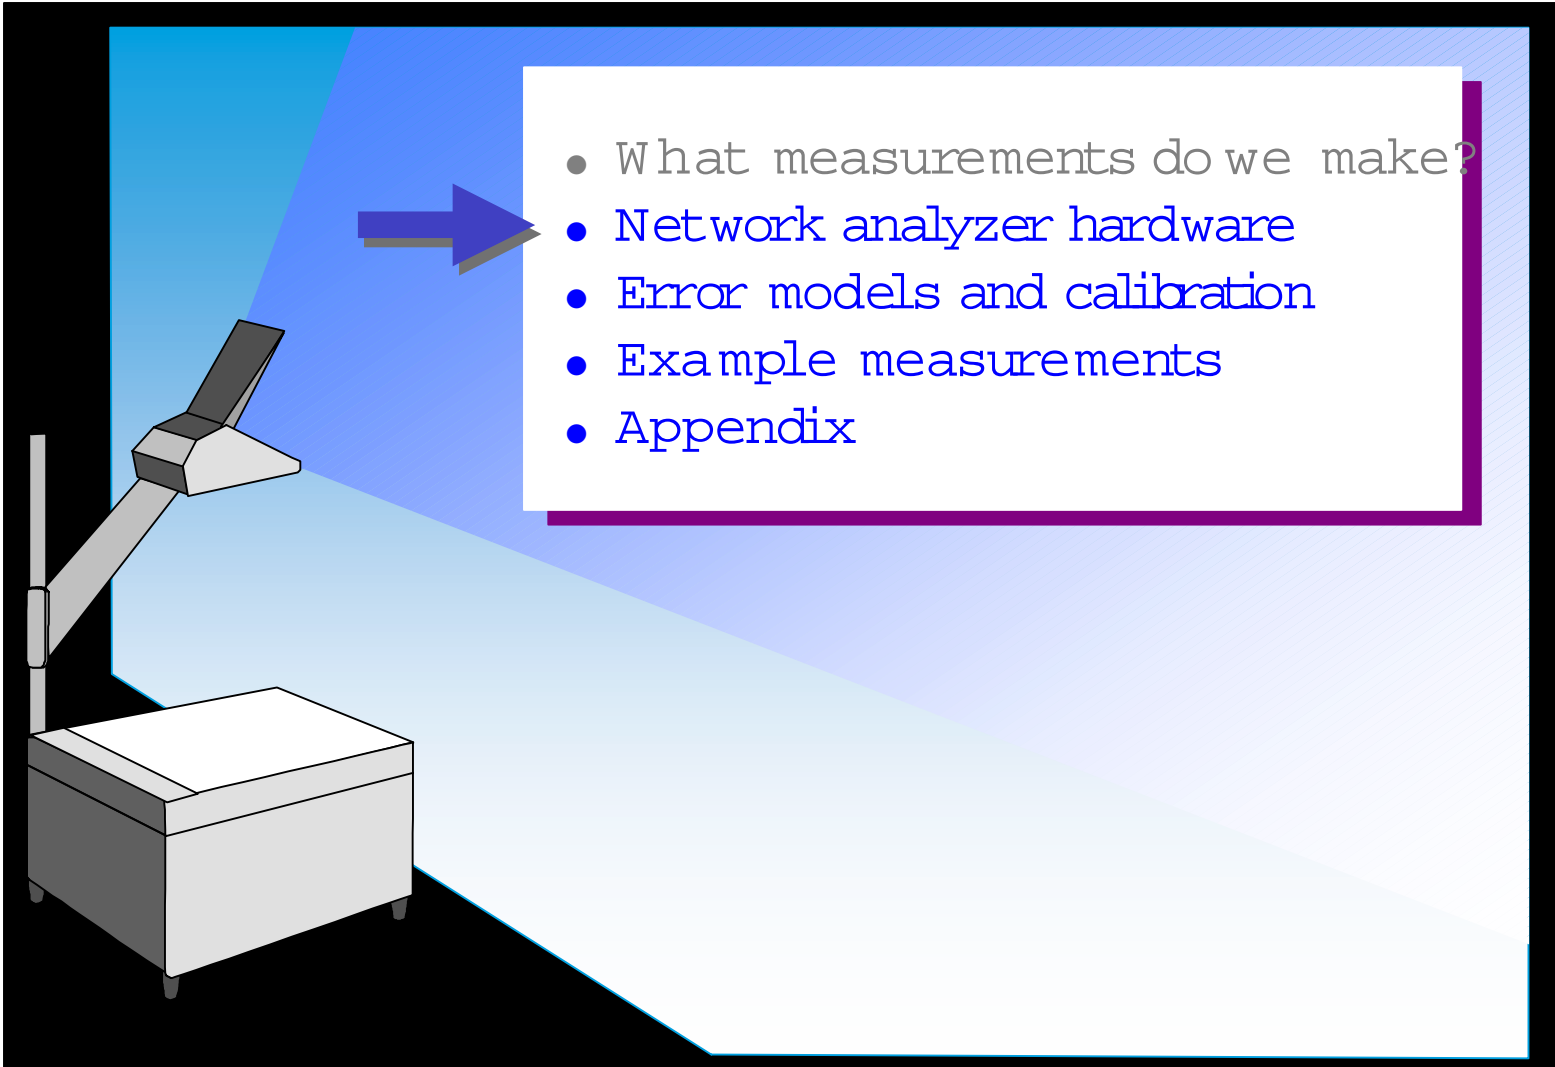- 
- What measurements do we make?
 - Network analyzer hardware
 - Error models and calibration
 - Example measurements
 - Appendix






Generalized Network Analyzer Block Diagram

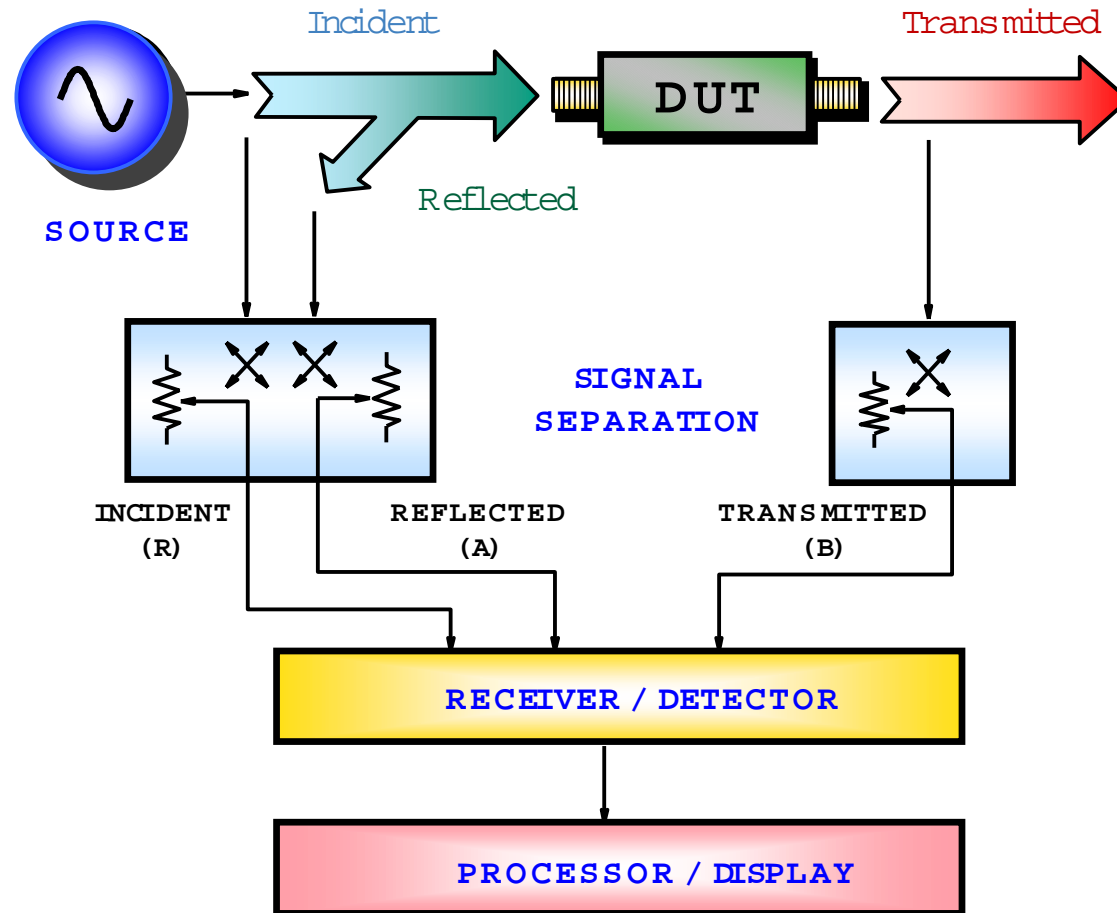





Source

- Supplies stimulus for system
- Swept frequency or power
- Traditionally NAs used separate source
- Most Agilent analyzers sold today have *integrated, synthesized* sources

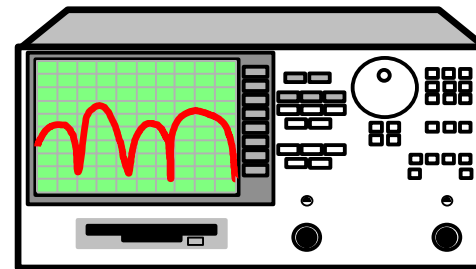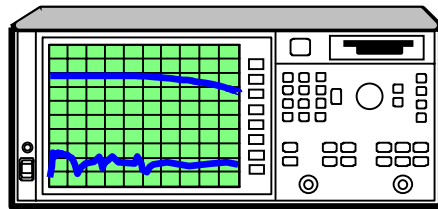


Signal Separation

- measure incident signal for reference
- separate incident and reflected signals

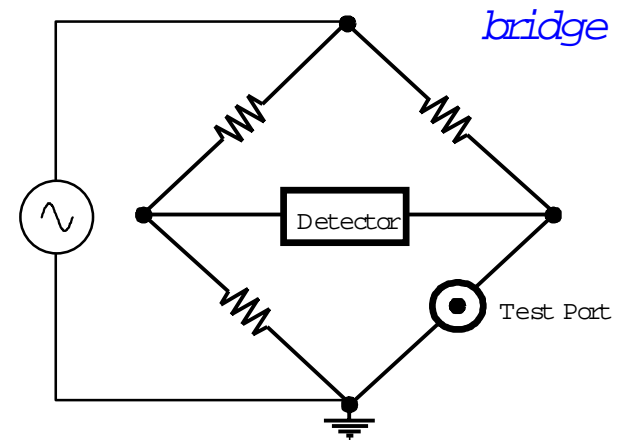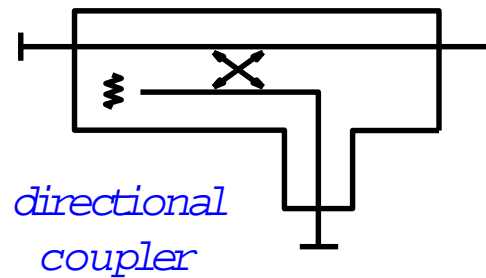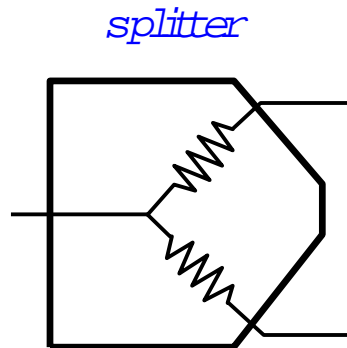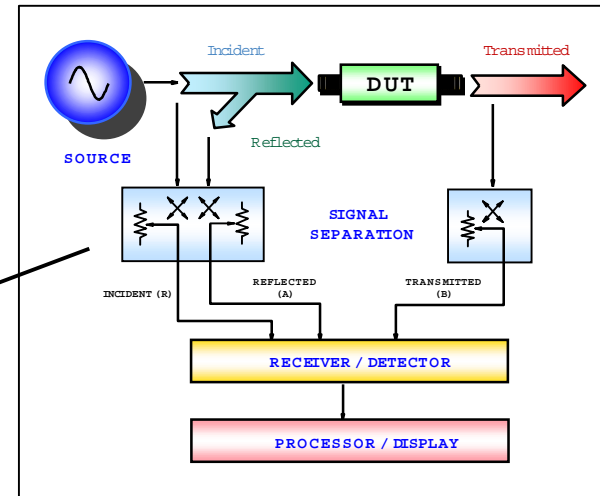


Directivity

Directivity is a measure of how well a coupler can separate signals moving in opposite directions

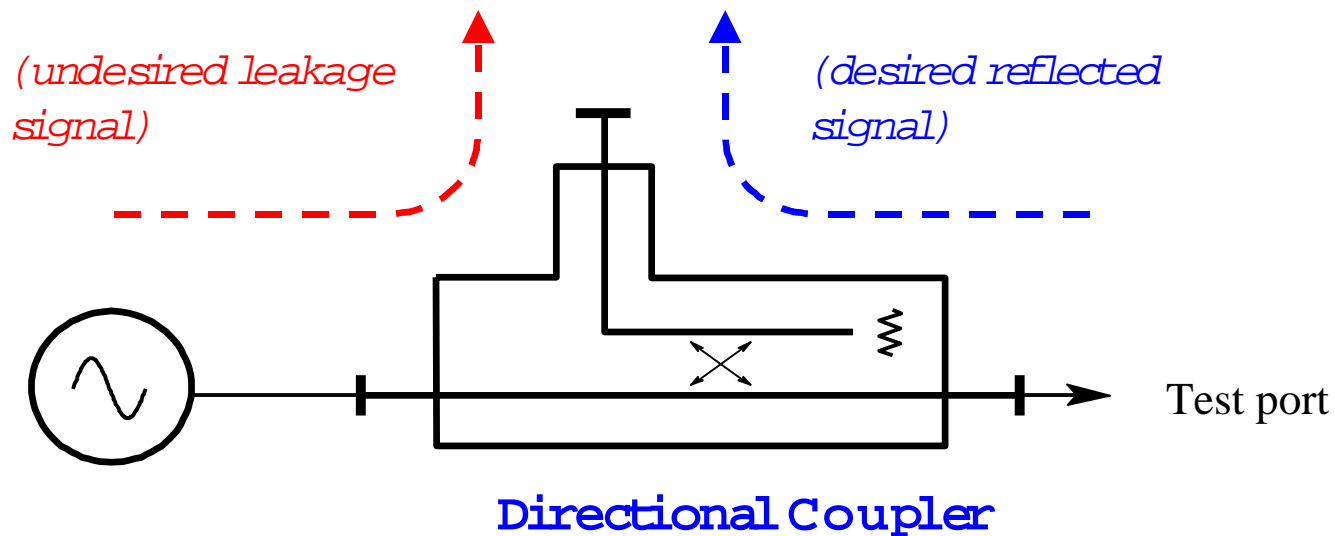

Interaction of Directivity with the DUT (Without Error Correction)

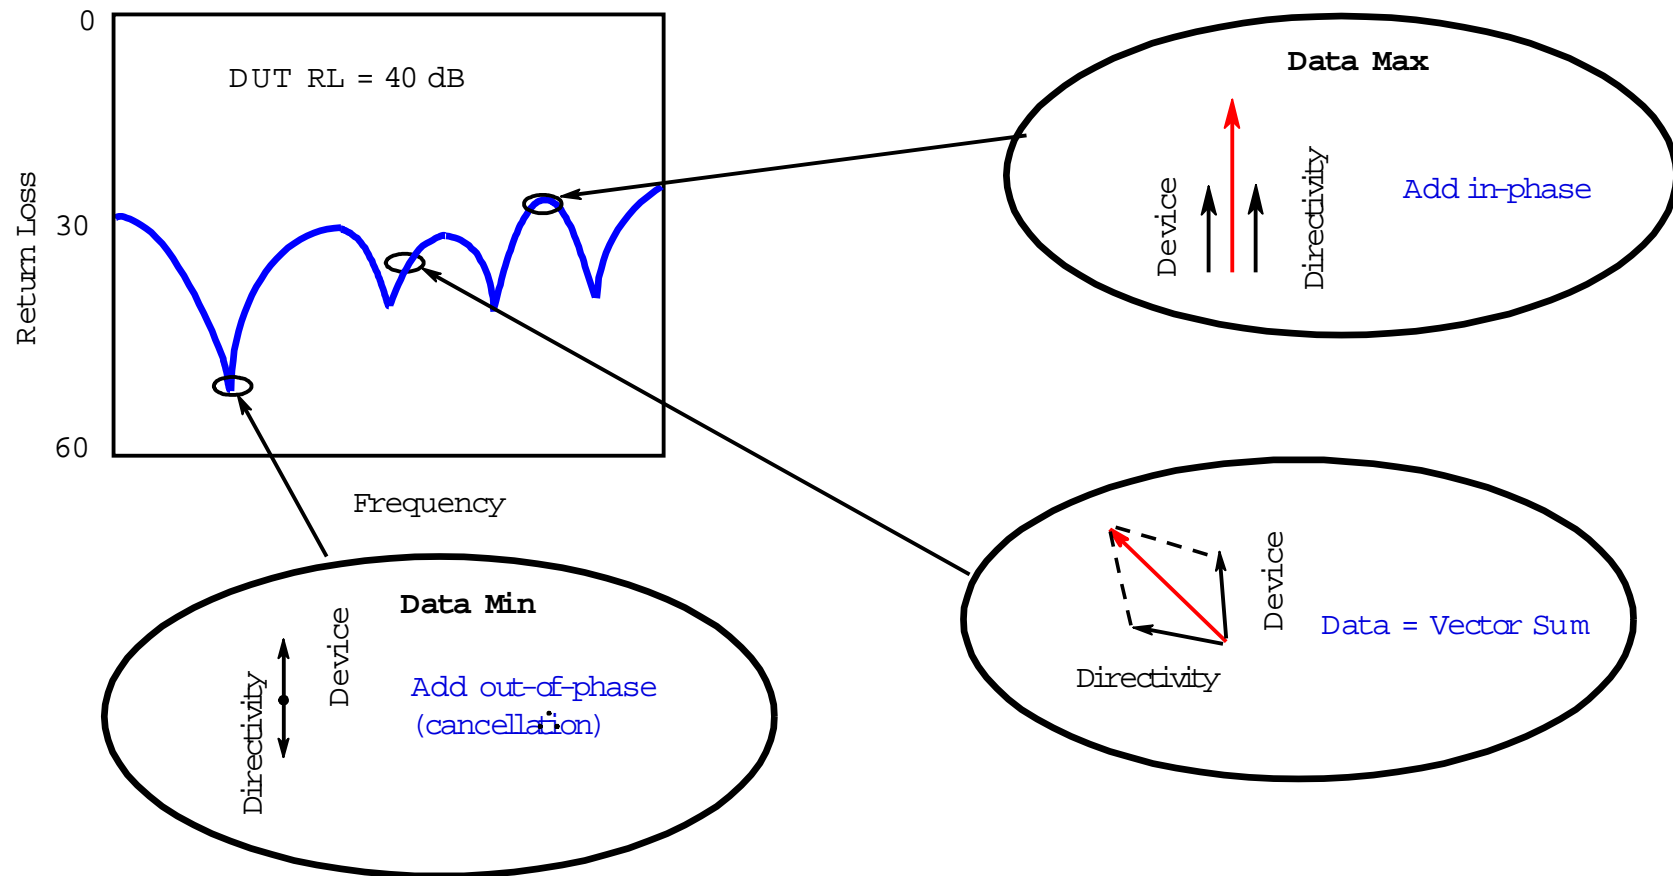


Detector Types

Diode





Scalar **broadband**

(no phase information)

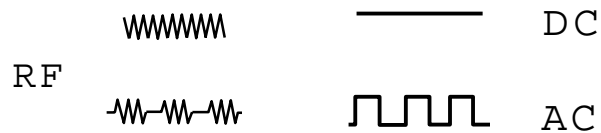


Tuned Receiver

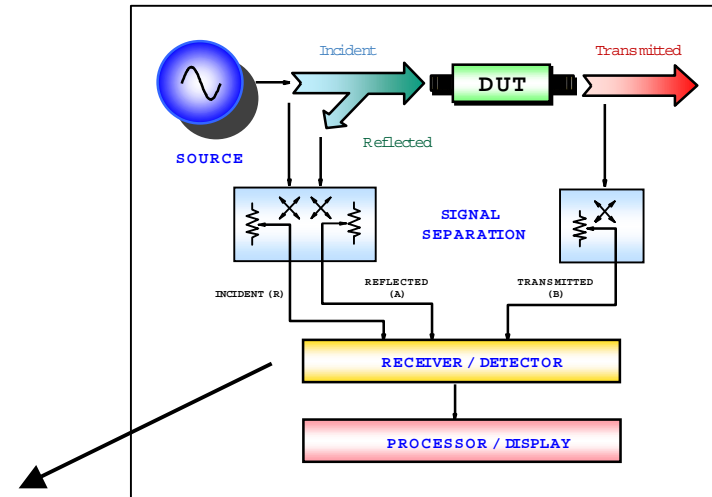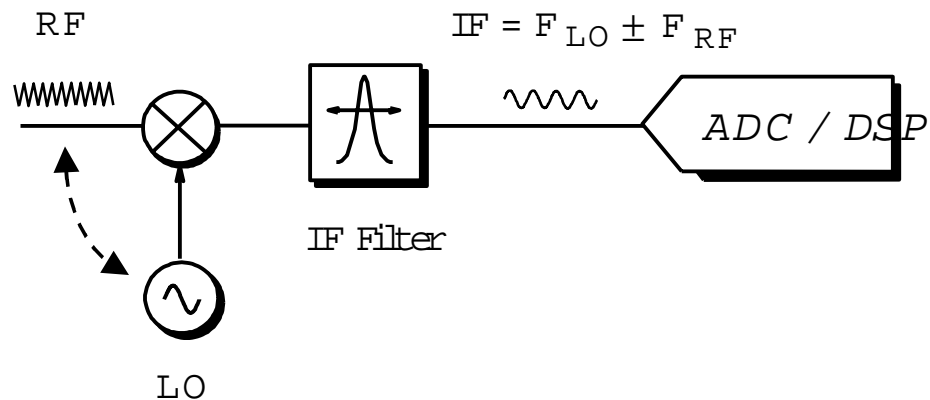


Vector
(magnitude and phase)




Broadband Diode Detection

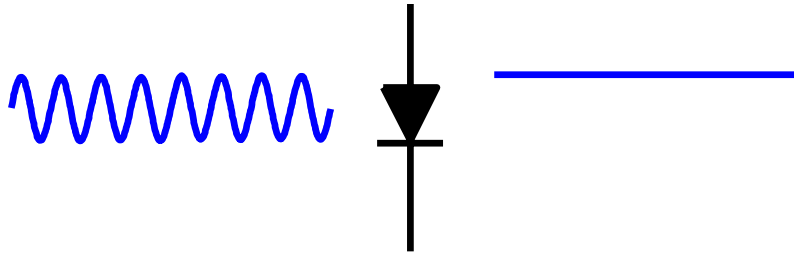


- Easy to make **broadband**
- **Inexpensive** compared to tuned receiver
- Good for measuring frequency-translating devices
- Improve dynamic range by increasing power
- **Medium** sensitivity / dynamic range

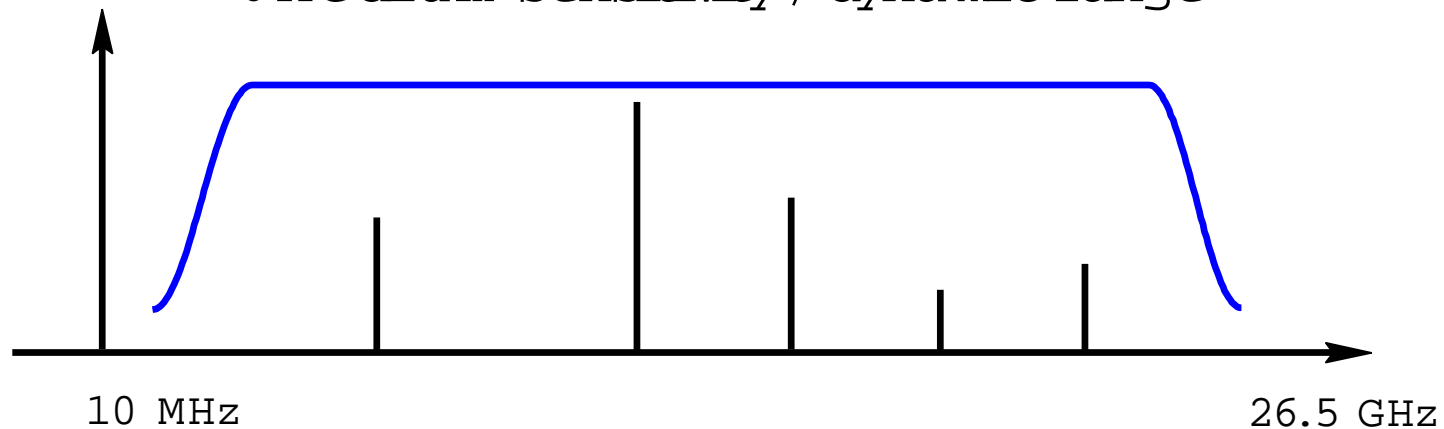

Narrowband Detection – Tuned Receiver

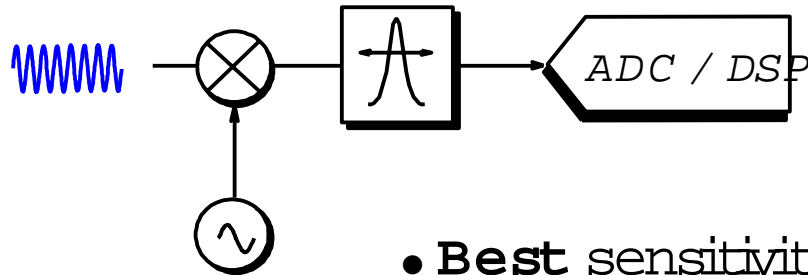


- **Best** sensitivity / dynamic range
- Provides harmonic / spurious signal **rejection**
- Improve dynamic range by increasing **power**, decreasing IF **bandwidth**, or **averaging**
- Trade off noise floor and measurement speed

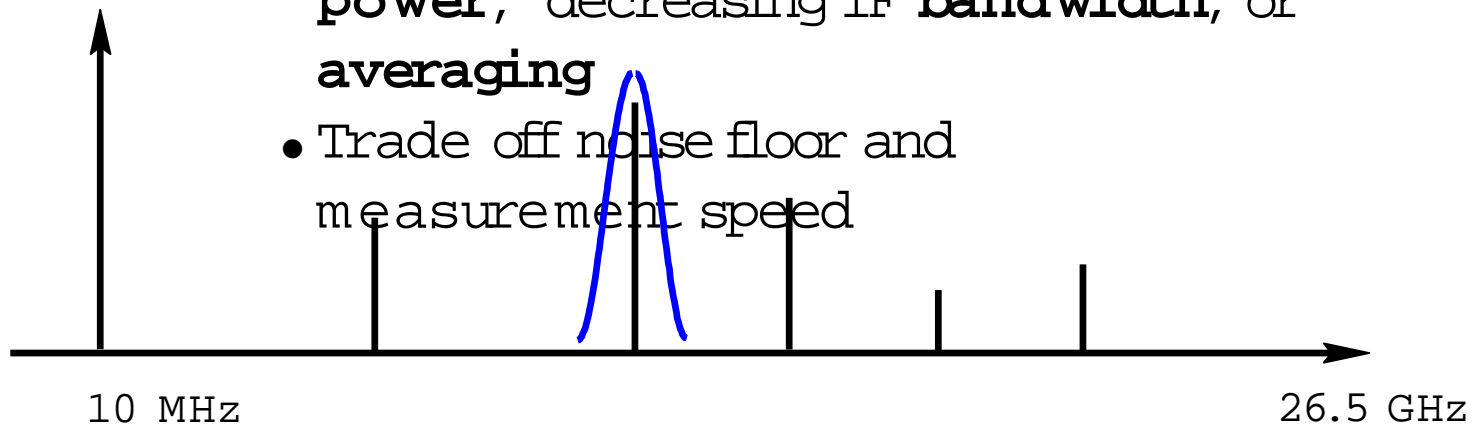

Comparison of Receiver Techniques

Broadband (diode)

detection

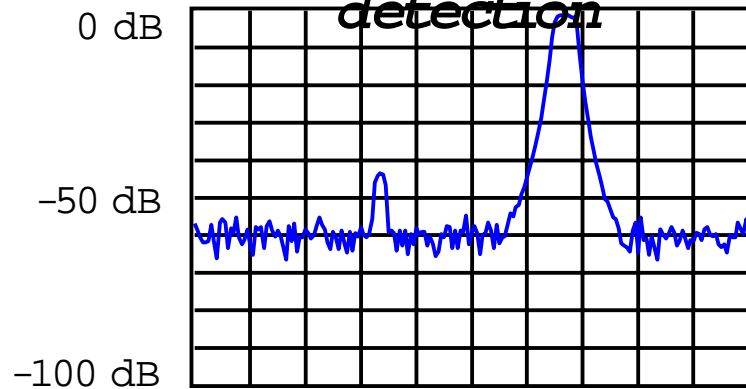


-60 dBm Sensitivity

- higher noise floor
- false responses

Narrowband (tuned-receiver)

detection

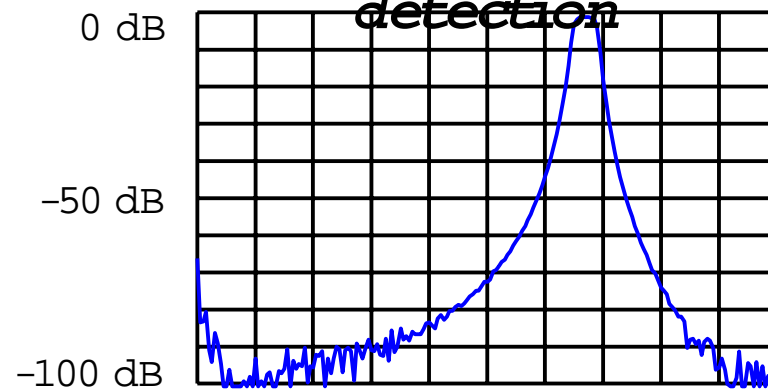


< -100 dBm Sensitivity

- high dynamic range
- harmonic immunity

*Dynamic range = maximum receiver power -
receiver noise floor*



Dynamic Range and Accuracy

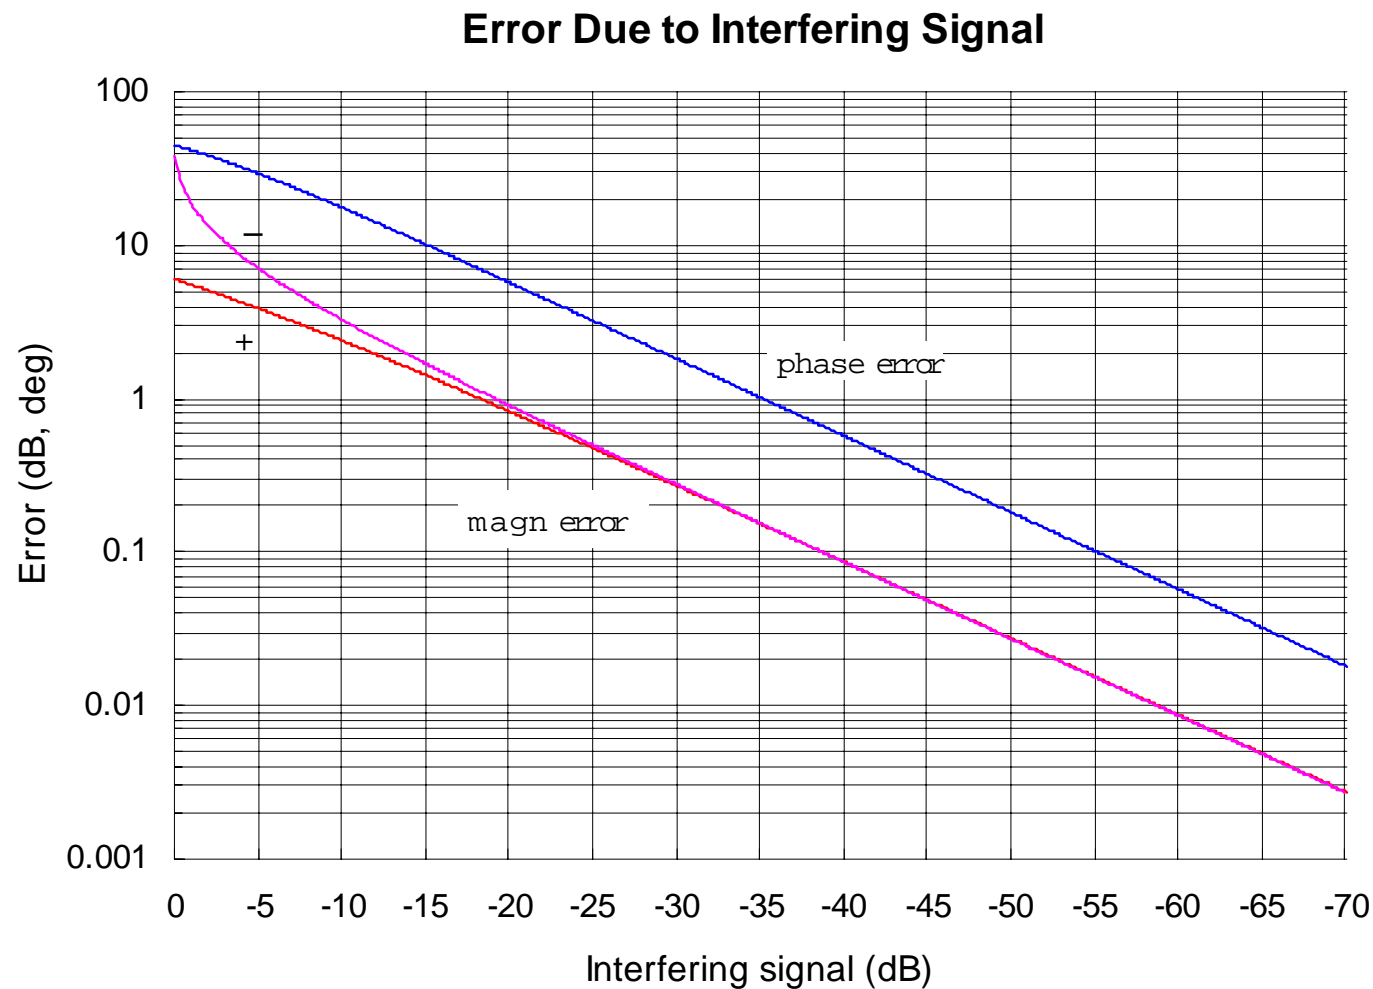


*Dynamic range
is very important
for measurement
accuracy!*



T/R Versus S-Parameter Test Sets

Transmission/Reflection Test Set

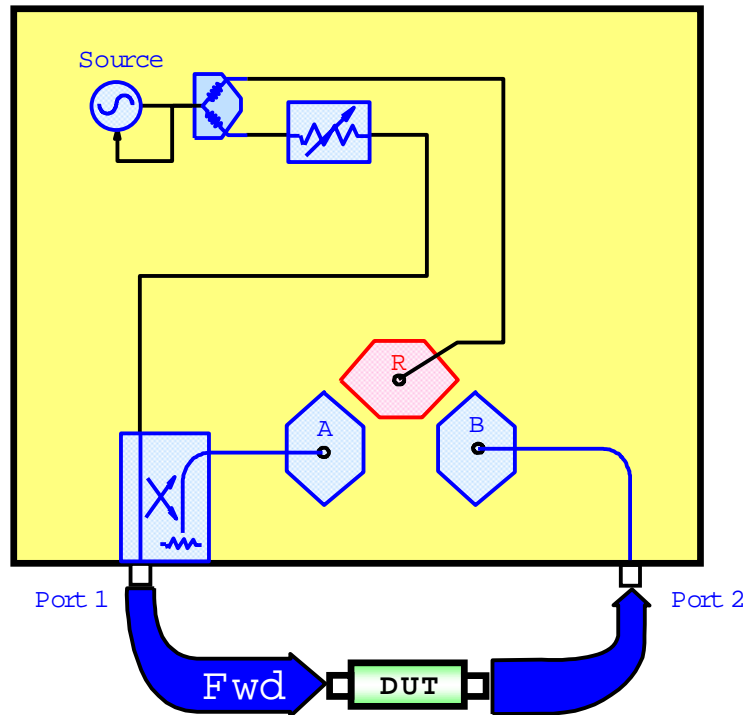


- RF always comes out port 1
- port 2 is always receiver
- **response, one-port cal**

Network Analyzer Basics
available



Agilent Technologies


S-Parameter Test Set

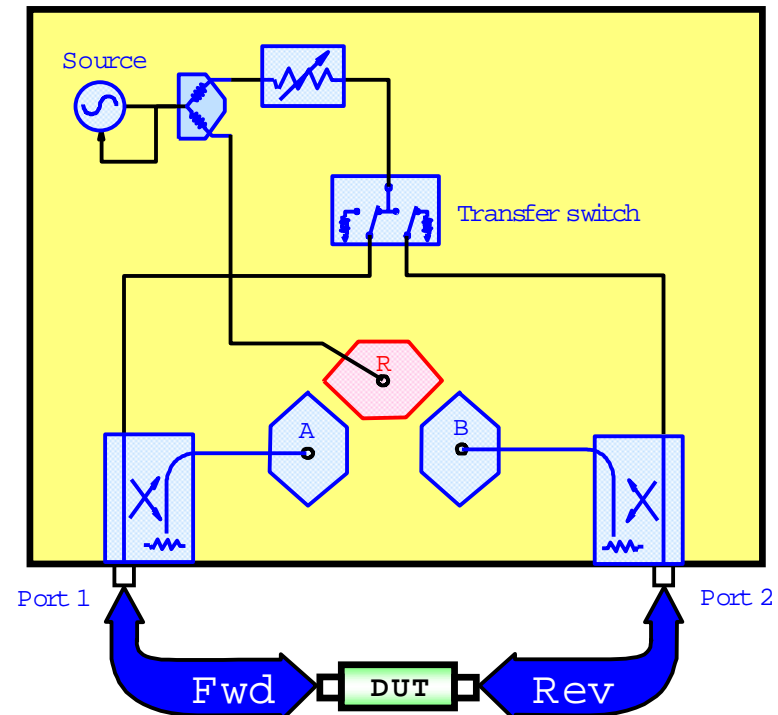


- RF comes out port 1 or port 2
- forward and reverse measurements
- **two-port calibration**
- possible

Copyright
2000

Processor / Display

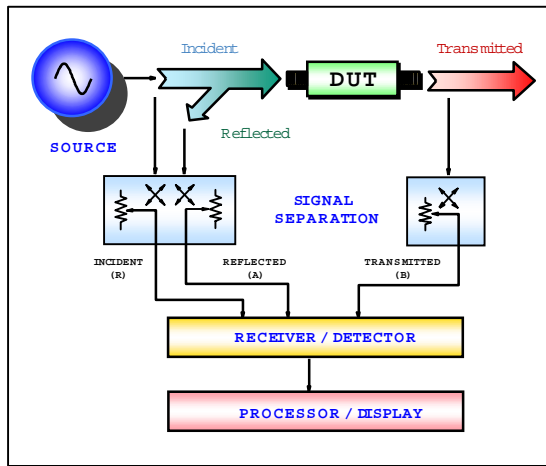

- markers
- limit lines
- pass/fail indicators
- linear/log formats
- grid/polar/Smith charts

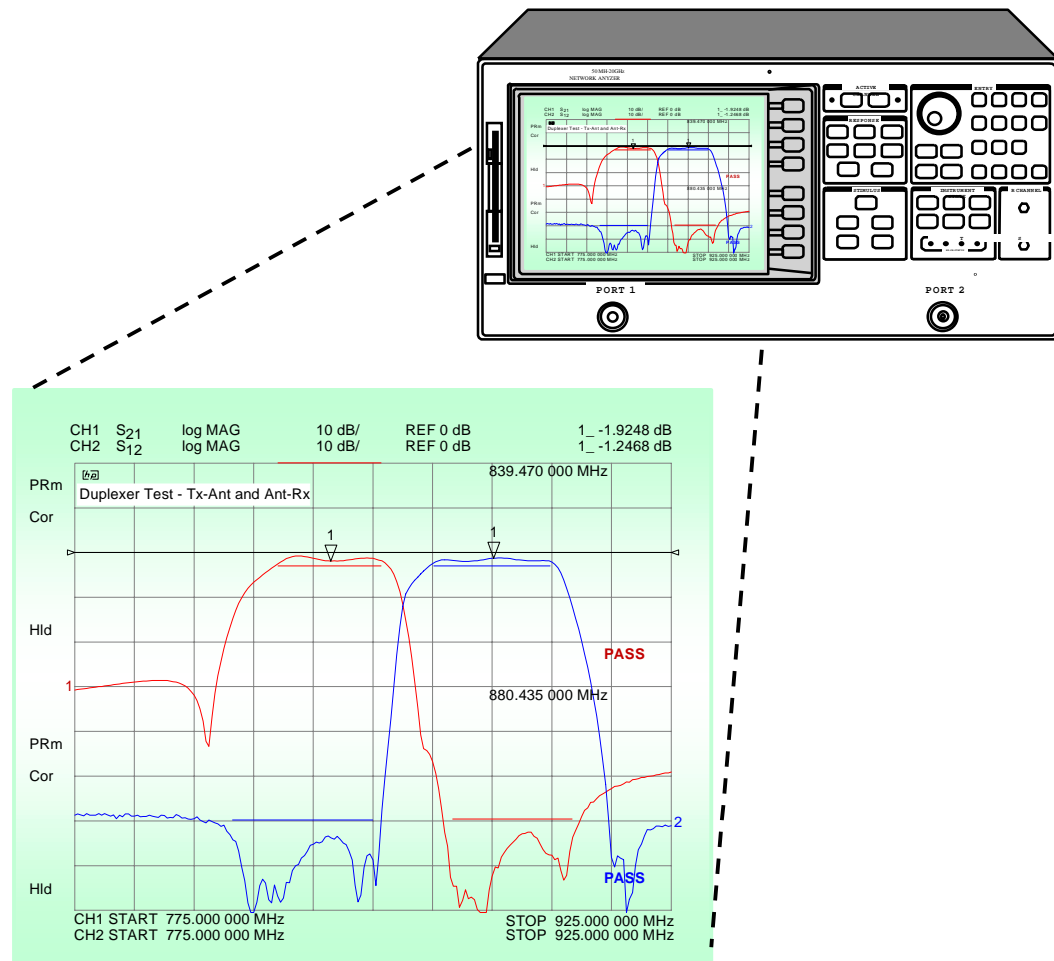

Internal Measurement Automation

Simple: **recall states**

More powerful:

- **Test sequencing**

- available on 8753/ 8720 families
- keystroke recording
- some advanced functions

- **IBASIC**

- available on 8712 family
- sophisticated programs
- custom user interfaces

ABCDEFGHIJKLMNOPQRSTUVWXYZ0123456789 + - / * = < > () & " ' , . / ? ; : ' []

```
1 ASSIGN @Hp8714 TO 800
2 OUTPUT @Hp8714;"SYST:PRES; *WAI"
3 OUTPUT @Hp8714;"ABOR;:INIT1:CONT OFF;*WAI"
4 OUTPUT @Hp8714;"DISP:ANN:FREQ1:MODE SSTOP"
5 OUTPUT @Hp8714;"DISP:ANN:FREQ1:MODE CSPAN"
6 OUTPUT @Hp8714;"SENS1:FREQ:CEN 175000000 HZ;*WAI"
7 OUTPUT @Hp8714;"ABOR;:INIT1:CONT OFF;:INIT1;*WAI"
8 OUTPUT @Hp8714;"DISP:WIND1:TRAC:Y:AUTO ONCE"
9 OUTPUT @Hp8714;"CALC1:MARK1 ON"
10 OUTPUT @Hp8714;"CALC1:MARK:FUNC BWID"
11 OUTPUT @Hp8714;"SENS2:STAT ON; *WAI"
12 OUTPUT @Hp8714;"SENS2:FUNC 'XFR:POW:RAT 1,0';DET NBAN; *WAI"
13 OUTPUT @Hp8714;"ABOR;:INIT1:CONT OFF;:INIT1;*WAI"
14 OUTPUT @Hp8714;"DISP:WIND2:TRAC:Y:AUTO ONCE"
15 OUTPUT @Hp8714;"ABOR;:INIT1:CONT ON;*WAI"
16 END
```




Agilent's Series of HF Vector Analyzers

Microwave



8720ET/ES series

- 13.5, 20, 40 GHz
- economical
- fast, small, integrated
- test mixers, high-power amps

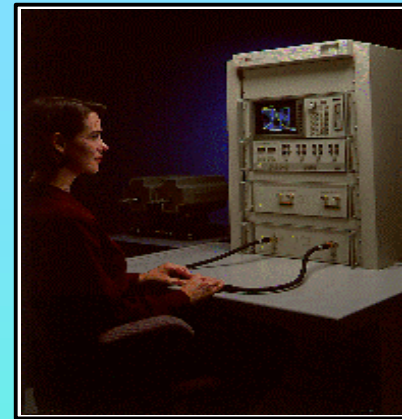

8510C series

- 110 GHz in coax
- highest accuracy
- modular, flexible
- pulse systems
- Tx/Rx module test

RF



8712ET/ES series

- 1.3, 3 GHz
- low cost
- narrowband and broadband detection
- IBASIC / LAN




8753ET/ES series

- 3, 6 GHz
- highest RF accuracy
- flexible hardware
- more features
- Offset and harmonic RF



Agilent's LF/RF Vector Analyzers

Combination NA / SA

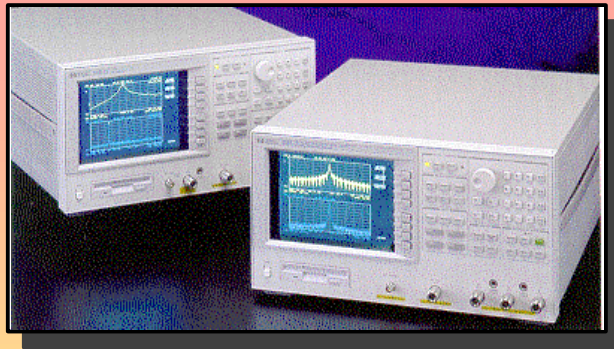

4395A/4396B

- 500 MHz (4395A), 1.8 GHz (4396B)
- impedance-measuring option
- fast, FFT-based spectrum analysis
- time-gated spectrum-analyzer option
- IBASIC
- standard test fixtures

LF




E5100A/B

- 180, 300 MHz
- economical
- fast, small
- target markets: crystals, resonators, filters
- equivalent-circuit models
- evaporation-monitor-function option



Spectrum Analyzer / Tracking Generator

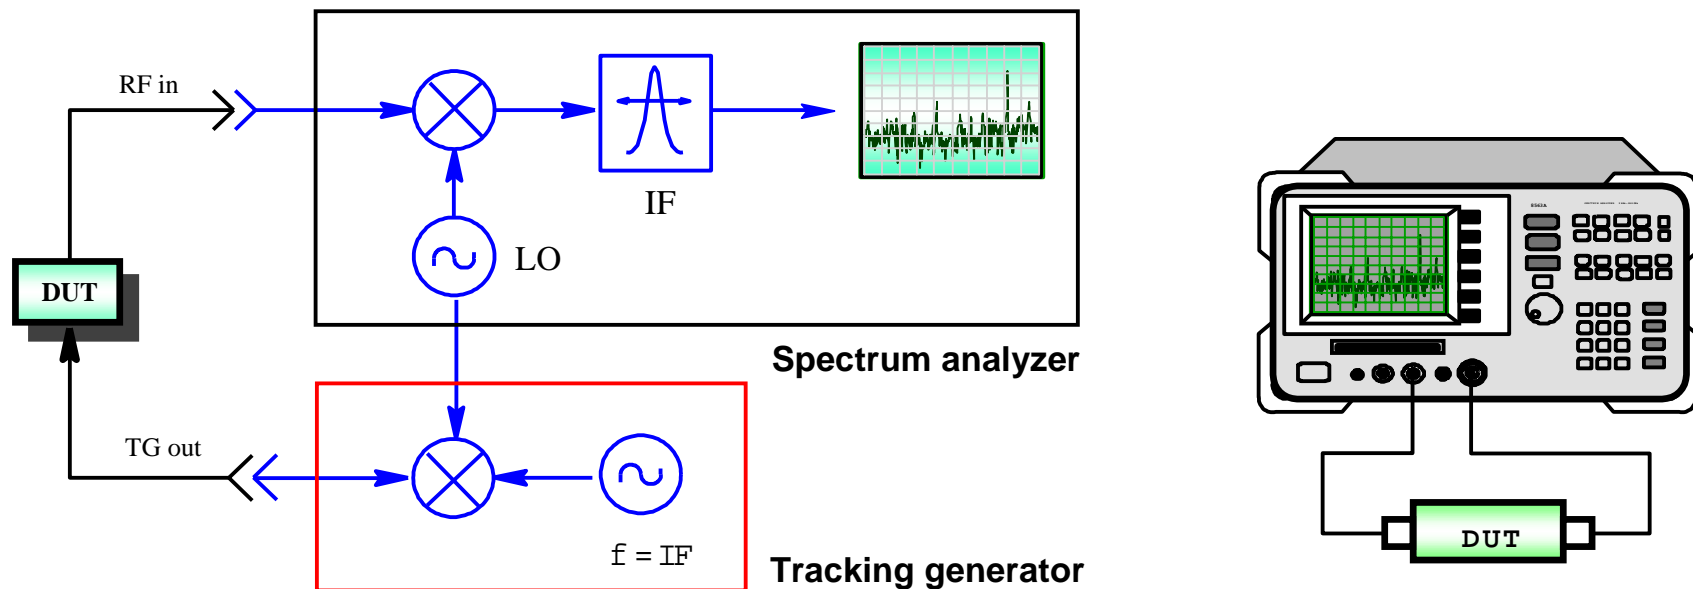


Key differences from network analyzer:

- **one channel** — no ratioed or phase measurements
- More **expensive** than scalar NA (but better dynamic range)
- Only error correction available is **normalization** (and possibly open-short averaging)
- Poorer **accuracy**
- Small **incremental cost** if SA is required for other measurements



Agenda

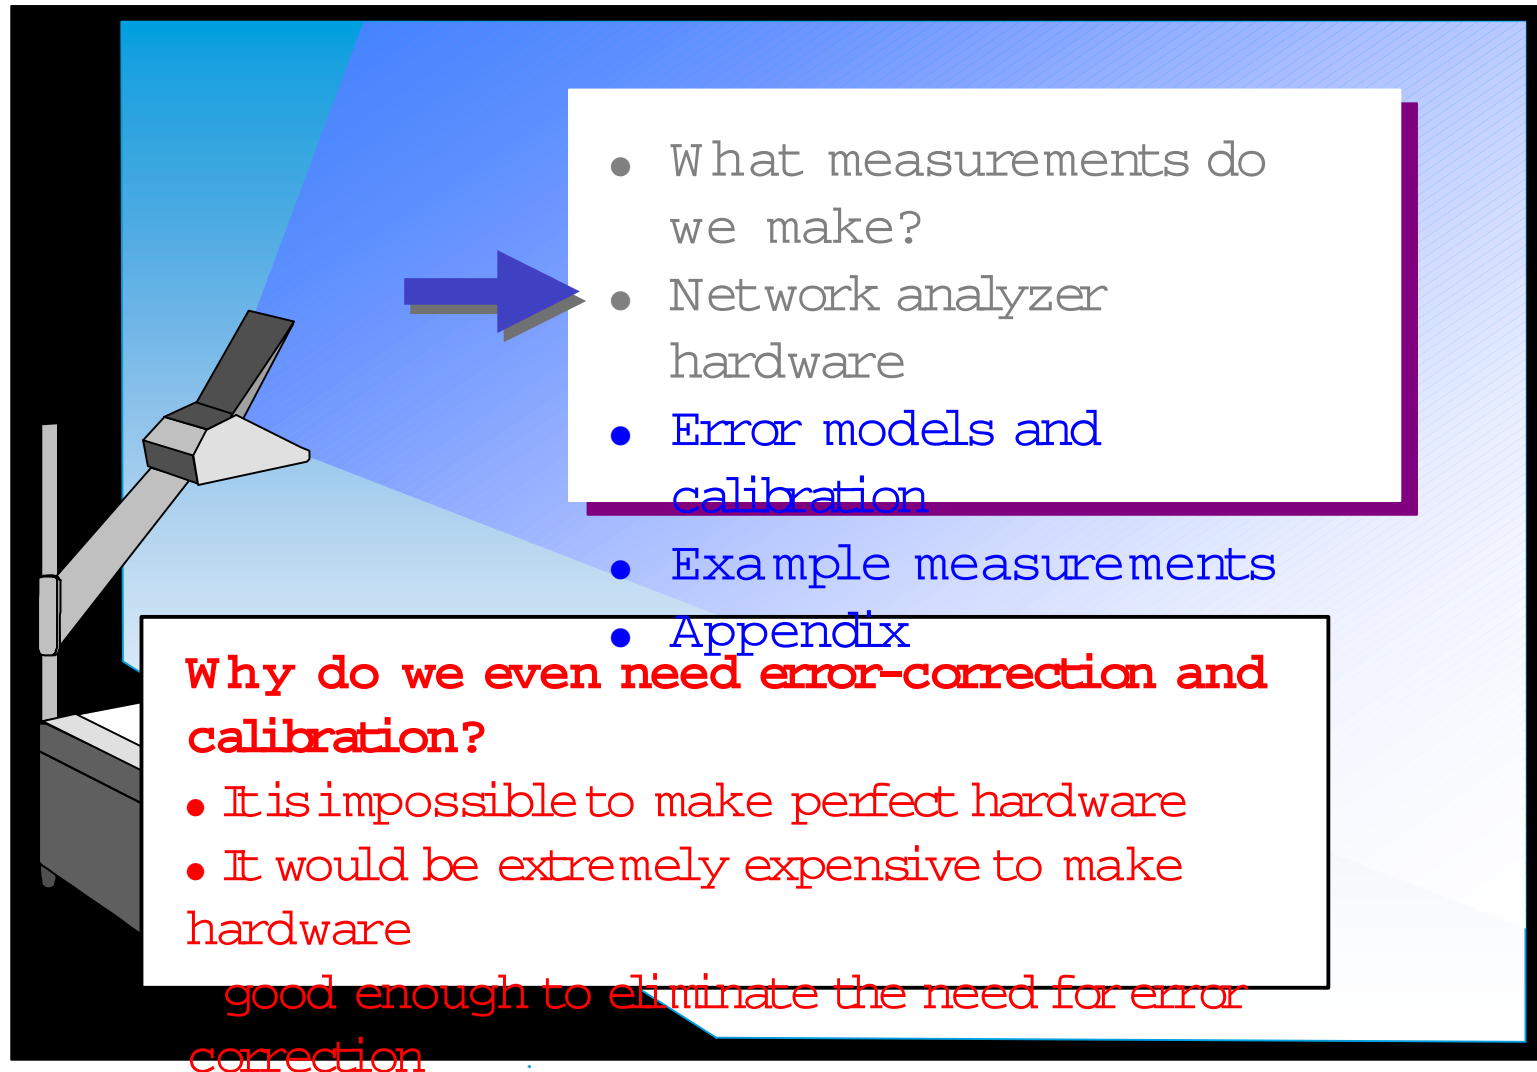


- What measurements do we make?
- Network analyzer hardware
- Error models and calibration
- Example measurements
- Appendix

Why do we even need error-correction and calibration?

- It is impossible to make perfect hardware
- It would be extremely expensive to make hardware good enough to eliminate the need for error correction



Calibration Topics

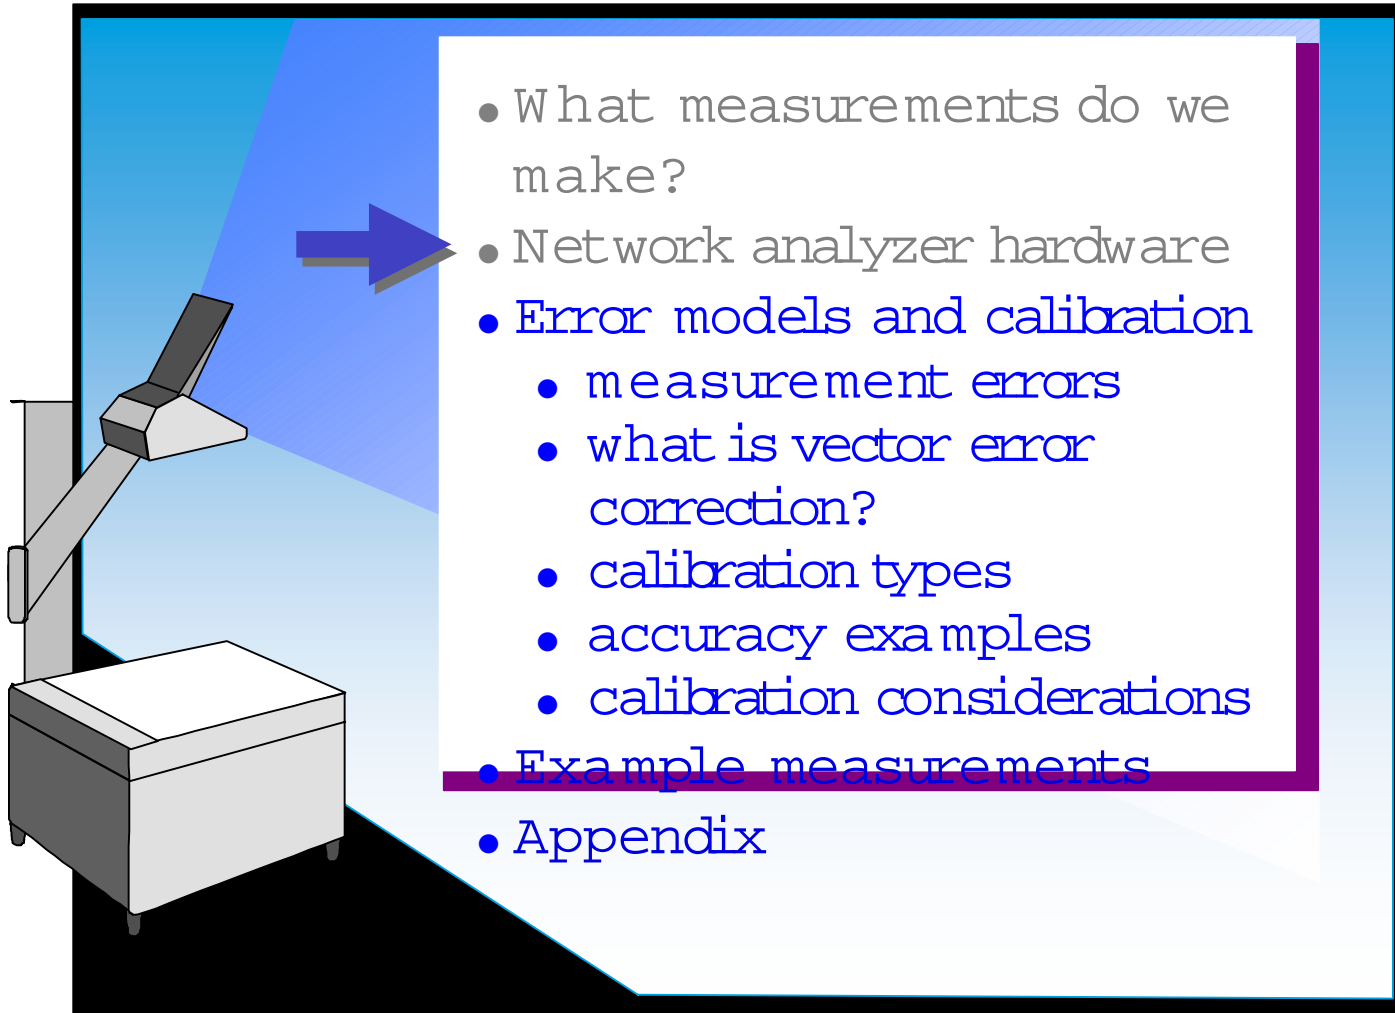

A stylized illustration of a network analyzer on the left, with a probe arm extending towards a large white rectangular box on the right. A blue arrow points from the probe towards the box. The box contains a bulleted list of calibration topics. The background of the slide features a blue and white geometric design.

- What measurements do we make?
- Network analyzer hardware
- Error models and calibration
 - measurement errors
 - what is vector error correction?
 - calibration types
 - accuracy examples
 - calibration considerations
- Example measurements
- Appendix



Measurement Error Modeling



Systematic errors

- due to **imperfections** in the analyzer and test setup
- assumed to be **time invariant** (predictable)




Random errors

- **vary** with time in random fashion (unpredictable)
- main contributors: instrument **noise**, switch and connector **repeatability**




Drift errors

- due to system performance changing **after** a calibration has been done
- primarily caused by **temperature variation**

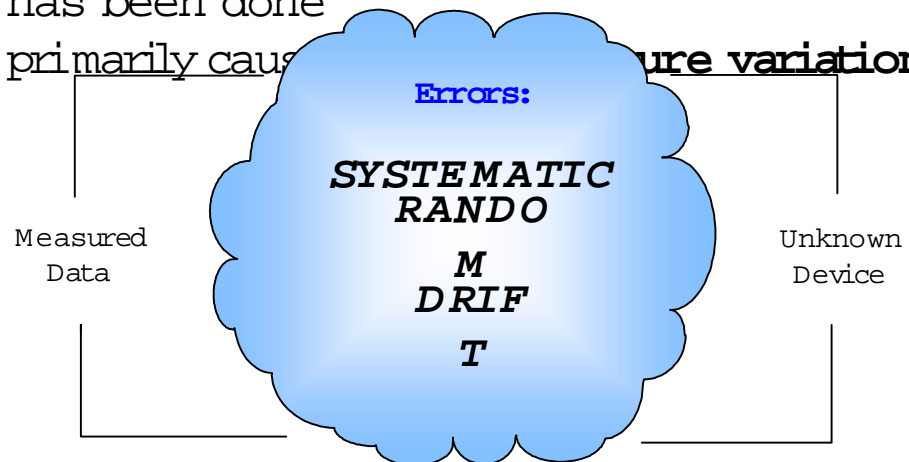

Systematic Measurement Errors

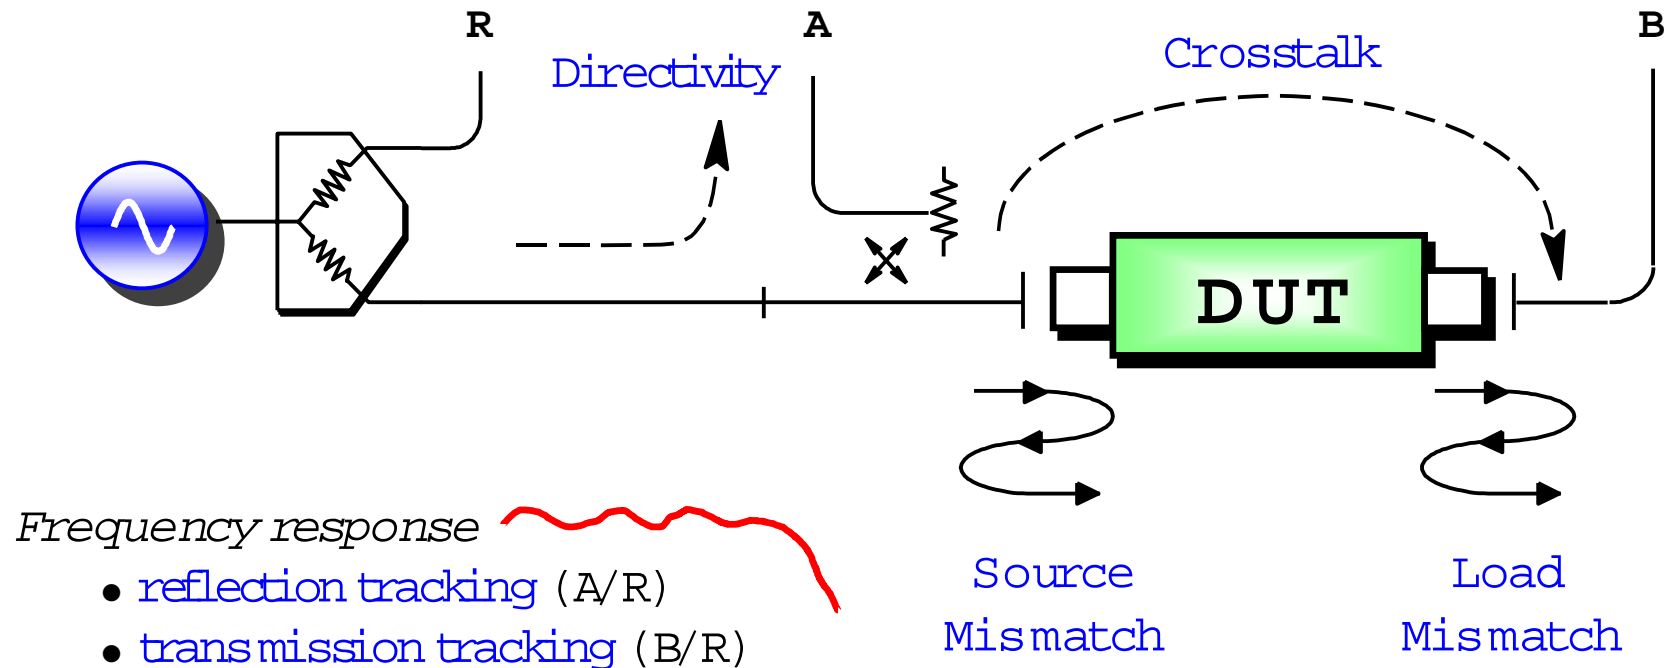

Six forward and six reverse error terms yields 12 error terms for two-port devices



Types of Error Correction



- **response (normalization)**

- simple to perform
- only corrects for tracking errors
- stores reference trace in memory, then does data divided by memory



- **vector**

- requires more standards
- requires an analyzer that can measure phase
- accounts for all major sources of systematic error

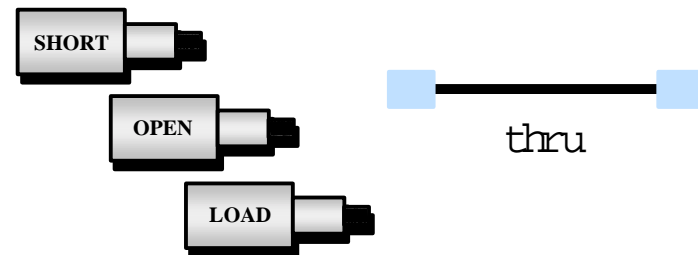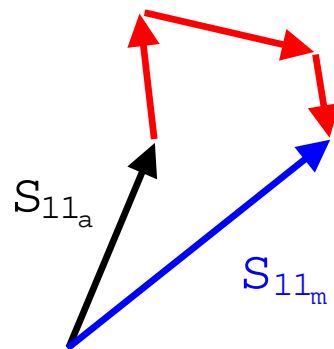


What is Vector-Error Correction?

- Process of characterizing systematic error terms
 - measure **known standards**
 - remove effects from subsequent measurements
- **1-port calibration** (*reflection measurements*)
 - only 3 systematic error terms measured
 - directivity, source match, and reflection tracking
- **Full 2-port calibration** (*reflection and transmission measurements*)
 - 12 systematic error terms measured
 - usually requires 12 measurements on four known standards (SOLT)
- Standards defined in **cal kit definition** file
 - network analyzer contains standard cal kit definitions
 - **CAL KIT DEFINITION MUST MATCH ACTUAL CAL KIT USED!**
- User-built standards must be characterized and entered into user cal kit



Reflection: One-Port Model

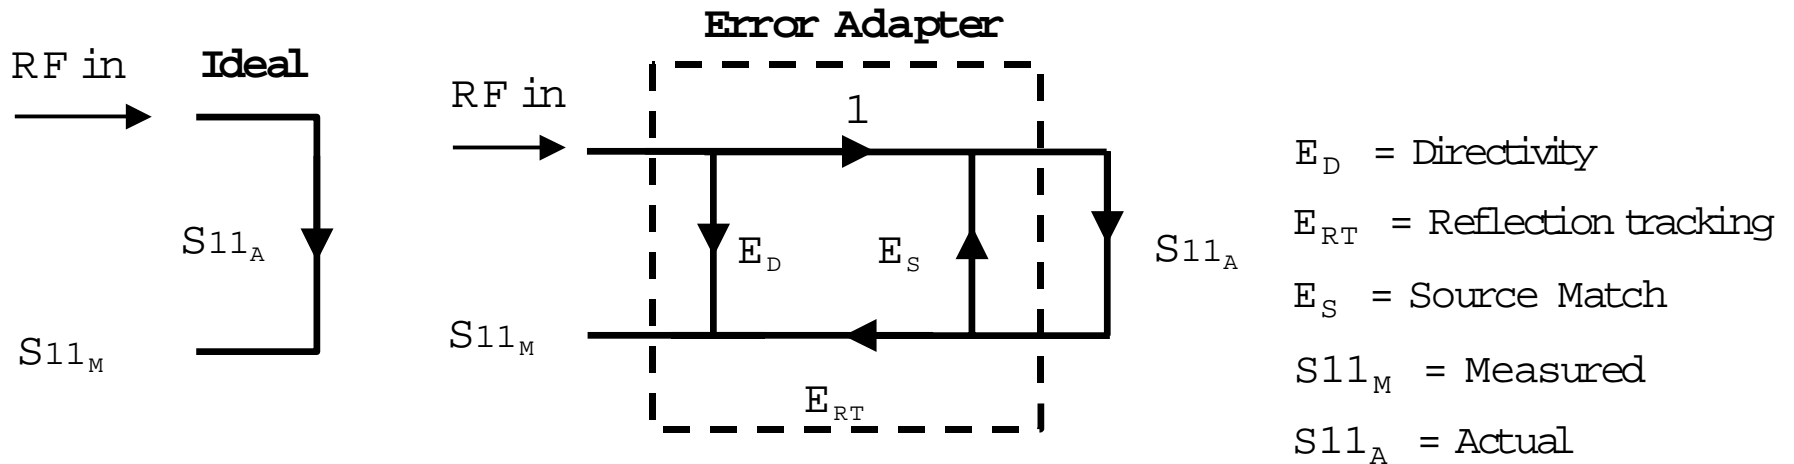


To solve for error terms,
we measure 3 standards
to generate 3 equations
and 3 unknowns

$$S_{11_M} = E_D + \frac{E_{RT} S_{11_A}}{1 - E_S S_{11_A}}$$

- Assumes good termination at port two if testing two-port devices
- If using port 2 of NA and DUT reverse isolation is low (e.g., filter passband):
 - assumption of good termination is not valid
 - two-port error correction yields better results




Before and After One-Port Calibration

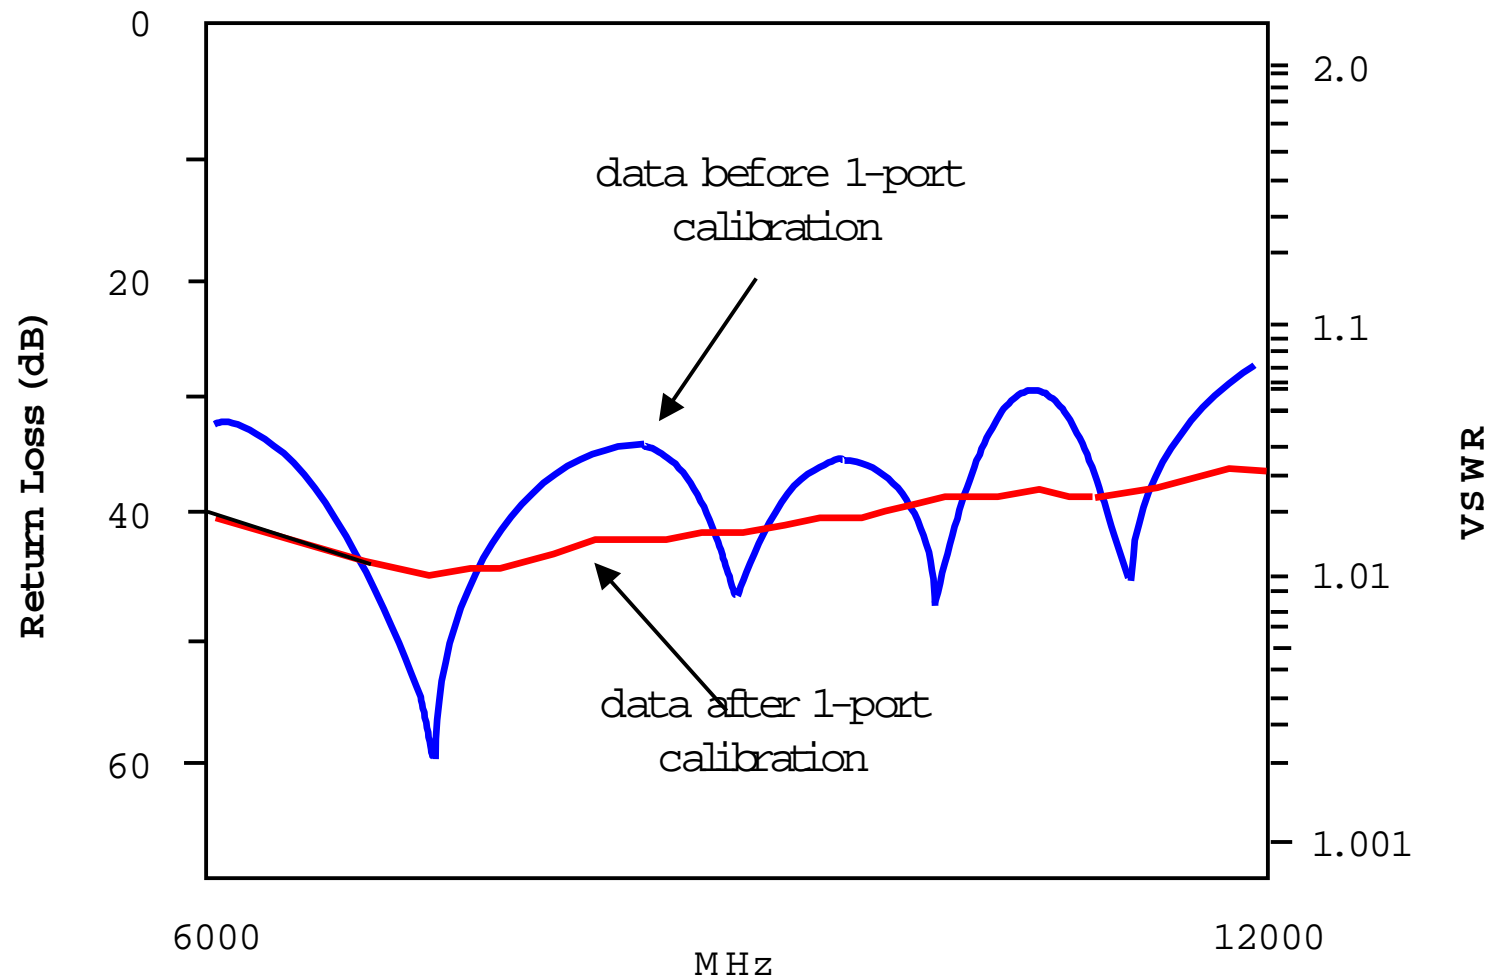


Two-Port Error Correction

Forward model

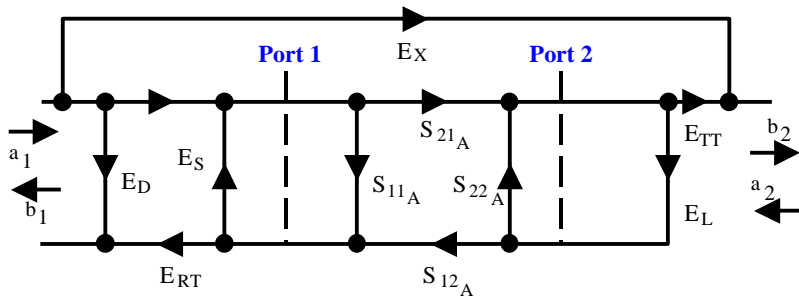

Reverse model

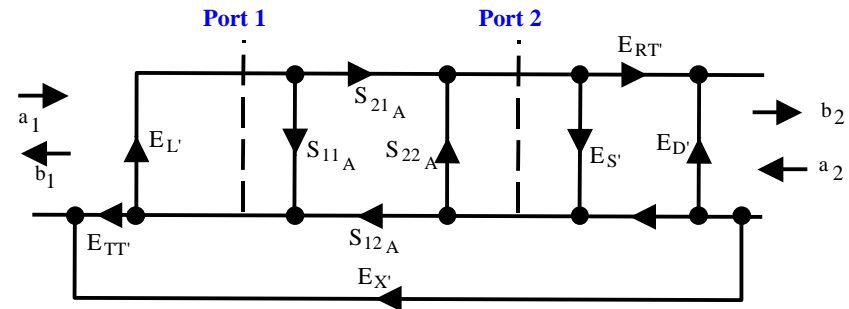

E_D = fwd directivity	E_L = fwd load match
E_S = fwd source match	E_{TT} = fwd transmission tracking
E_{RT} = fwd reflection tracking	E_X = fwd isolation
$E_{D'}$ = rev directivity	$E_{L'}$ = rev load match
$E_{S'}$ = rev source match	$E_{TT'}$ = rev transmission tracking
$E_{RT'}$ = rev reflection tracking	$E_{X'}$ = rev isolation

- Each actual S-parameter is a function of all four measured S-parameters
- Analyzer must make forward *and* reverse sweep to update any one S-parameter
- Luckily, you don't need to know

these equations to use network analyzers!!!

$$S_{11a} = \frac{\left(\frac{S_{11m} - E_D}{E_{RT}}\right)\left(1 + \frac{S_{22m} - E_{D'}}{E_{RT'}} E_{S'}\right) - E_L \left(\frac{S_{21m} - E_X}{E_{TT}}\right) \left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)}{\left(1 + \frac{S_{11m} - E_D}{E_{RT}} E_S\right)\left(1 + \frac{S_{22m} - E_{D'}}{E_{RT'}} E_{S'}\right) - E_{L'} E_L \left(\frac{S_{21m} - E_X}{E_{TT}}\right) \left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)}$$

$$S_{21a} = \frac{\left(\frac{S_{21m} - E_X}{E_{TT}}\right)\left(1 + \frac{S_{22m} - E_{D'}}{E_{RT'}} (E_{S'} - E_L)\right)}{\left(1 + \frac{S_{11m} - E_D}{E_{RT}} E_S\right)\left(1 + \frac{S_{22m} - E_{D'}}{E_{RT'}} E_{S'}\right) - E_{L'} E_L \left(\frac{S_{21m} - E_X}{E_{TT}}\right) \left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)}$$



$$S_{12a} = \frac{\left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)\left(1 + \frac{S_{11m} - E_D}{E_{RT}} (E_S - E_{L'})\right)}{\left(1 + \frac{S_{11m} - E_D}{E_{RT}} E_S\right)\left(1 + \frac{S_{22m} - E_{D'}}{E_{RT'}} E_{S'}\right) - E_{L'} E_L \left(\frac{S_{21m} - E_X}{E_{TT}}\right) \left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)}$$

$$S_{22a} = \frac{\left(\frac{S_{22m} - E_{D'}}{E_{RT'}}\right)\left(1 + \frac{S_{11m} - E_D}{E_{RT}} E_S\right) - E_{L'} \left(\frac{S_{21m} - E_X}{E_{TT}}\right) \left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)}{\left(1 + \frac{S_{11m} - E_D}{E_{RT}} E_S\right)\left(1 + \frac{S_{22m} - E_{D'}}{E_{RT'}} E_{S'}\right) - E_{L'} E_L \left(\frac{S_{21m} - E_X}{E_{TT}}\right) \left(\frac{S_{12m} - E_{X'}}{E_{TT'}}\right)}$$

Crosstalk: Signal Leakage Between Test Ports During

Transmission

- Can be a problem with:
 - high-isolation devices (e.g., switch in open position)
 - high-dynamic range devices (some filter stopbands)
- Isolation calibration
 - adds noise to error model (measuring near noise floor of system)
 - only perform if really needed (use averaging if necessary)
 - if crosstalk is **independent** on I match, use two terminations
 - if **dependent** on I match, use two terminations
 - if **dependent** on I match, use two terminations

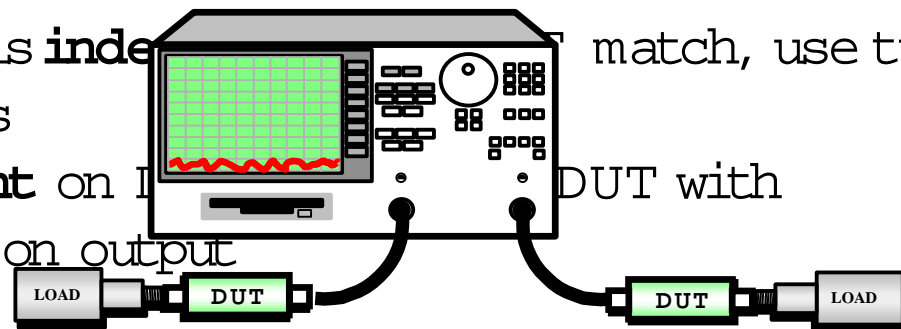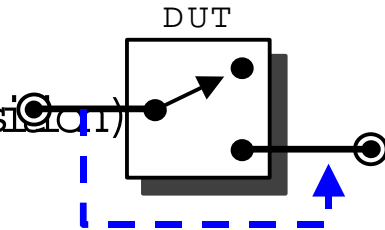


Errors and Calibration Standards

UNCORRECTED FULL 2-PORT



- Convenient
- Generally not accurate
- No errors removed

RESPONSE

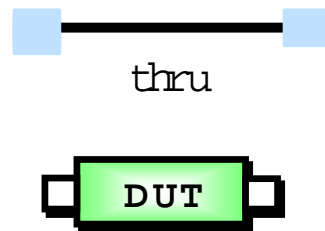


- Easy to perform
- Use when highest accuracy is not required
- Removes frequency response error



ENHANCED-RESPONSE

- Combines response and 1-port
- Corrects source match for transmission measurements

1-PORT

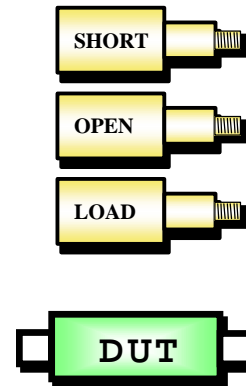

- For reflection measurements
- Need good termination for high accuracy with two-port devices
- Removes these errors:
 - Directivity
 - Source match
 - Reflection tracking

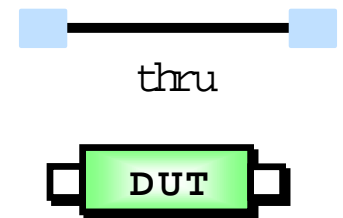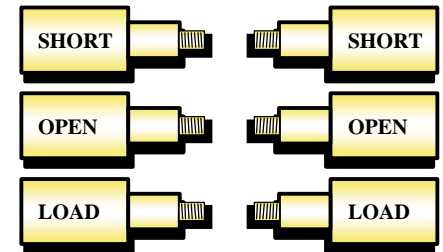

- Highest accuracy
- Removes these errors:
 - Directivity
 - Source, load match
 - Reflection tracking
 - Transmission tracking
 - Crosstalk




Calibration Summary

Reflection

Test Set (cal type)

	T/R (one-port)	S-parameter (two-port)
• Reflection tracking	✓	✓
• Directivity	✓	✓
• Source match	✓	
• Load match	✗	

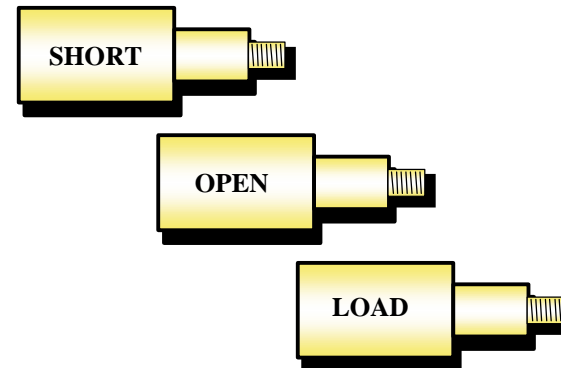

error can be corrected



error cannot be corrected



* *enhanced response cal corrects for source match during transmission measurements*


Transmission

Test Set (cal type)

	T/R (response, isolation)	S-parameter (two-port)
• Transmission Tracking	✓	✓
• Crosstalk	✓	✓
• Source match	✓*	✗
• Load match	✗	✓



Reflection Example Using a One-Port Cal

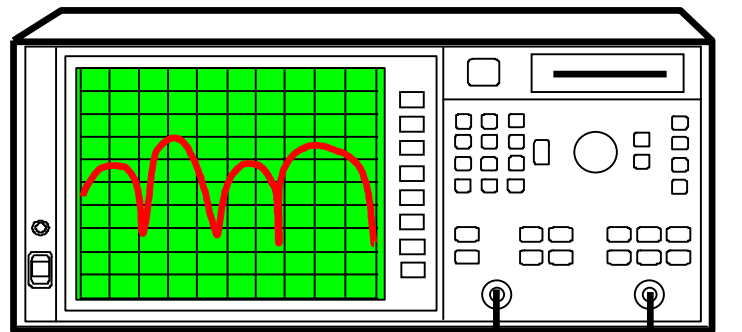

Directivity:
40 dB (.010)

.158

$$(.891)(.126)(.891) = .100$$

Load
match:
18 dB
(.126)

DUT

16 dB RL (.158)
1 dB loss (.891)

*Remember: convert all dB
values to linear for
uncertainty calculations!*

$$\rho \propto \text{loss}_{(\text{linear})}^{\frac{20}{10}} = 10$$


Measurement uncertainty:

$$\begin{aligned} & -20 * \log (.158 + .100 + .010) \\ & = 11.4 \text{ dB } \textbf{(-4.6dB)} \end{aligned}$$

$$\begin{aligned} & -20 * \log (.158 - .100 - .010) \\ & = 26.4 \text{ dB } \textbf{(+10.4 dB)} \end{aligned}$$



Using a One-Port Cal +

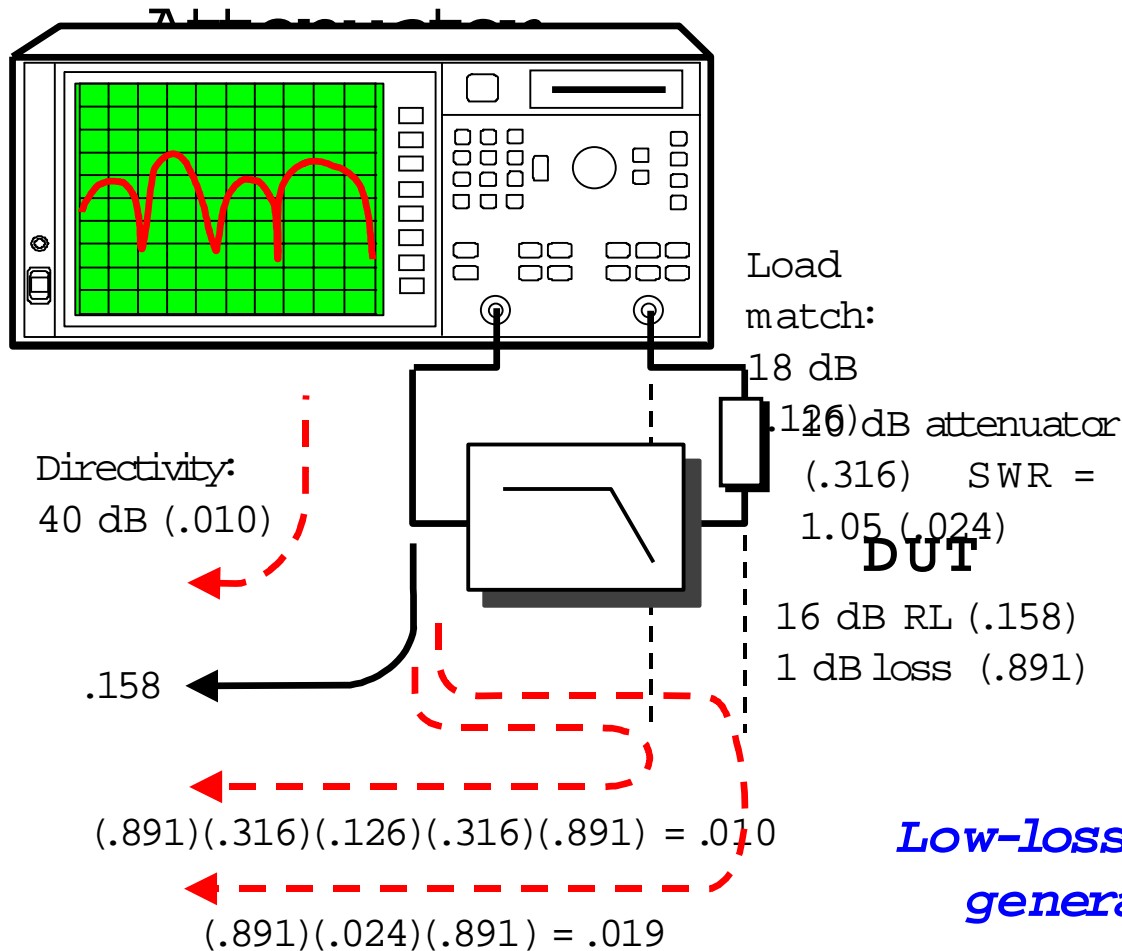

Measurement
uncertainty:

$$-20 * \log (.158 + .039)$$

$$= 14.1 \text{ dB } (-1.9 \text{ dB})$$

$$-20 * \log (.158 - .039)$$


$$= 18.5 \text{ dB } (+2.5 \text{ dB})$$

$$\text{Worst-case error} = .010 + .010 + .019 = .039$$

*Low-loss bi-directional devices
generally require two-port
calibration
for low measurement uncertainty*



Transmission Example Using Response Cal

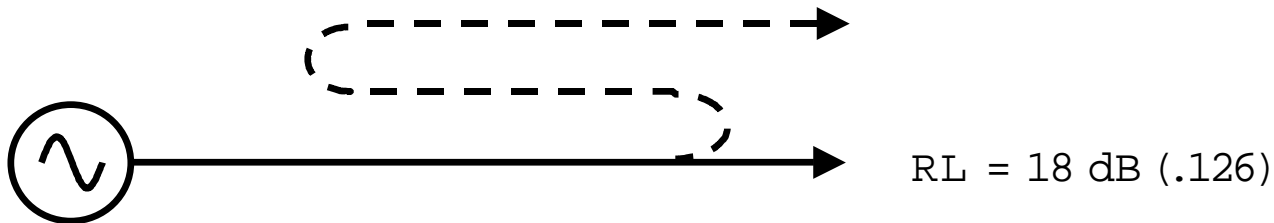

RL = 14 dB (.200)

Thru calibration (normalization) builds error into measurement due to source and load

match interaction

Calibration

Uncertainty


$$= (1 \pm \rho_s \rho_L)$$

$$= (1 \pm (.200)(.126))$$

$$= \pm 0.22 \text{ dB}$$



Filter Measurement with Response Cal

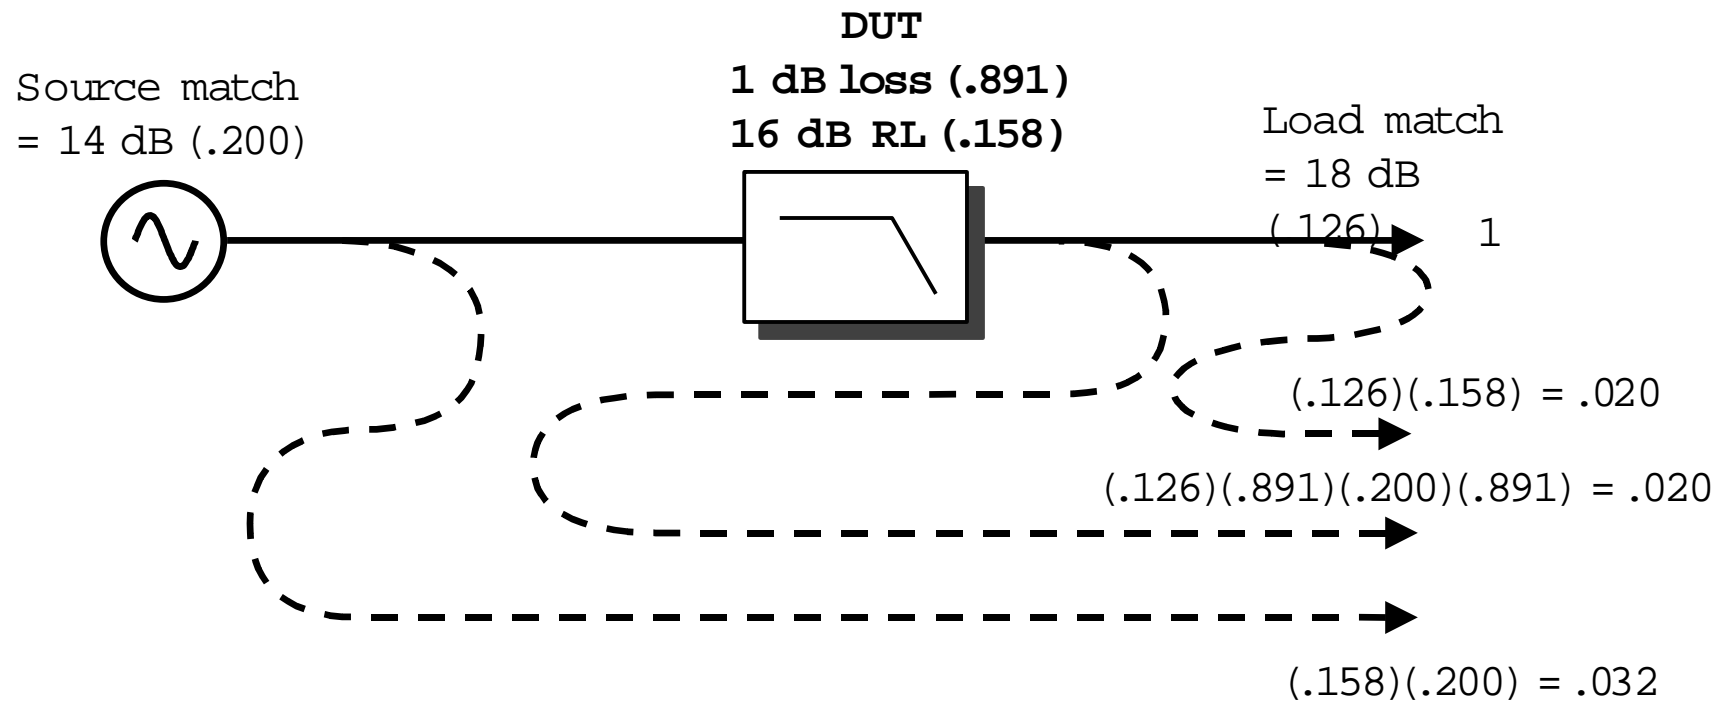

Total measurement uncertainty:

$$+0.60 + 0.22 = +0.82$$

dB

$$-0.65 - 0.22 = -0.87$$

dB


Measurement uncertainty

$$= 1 \pm (.020 + .020 + .032)$$


$$= 1 \pm .072$$

$$= +0.60 \text{ dB}$$

$$-0.65 \text{ dB}$$



Measuring Amplifiers with a Response Cal

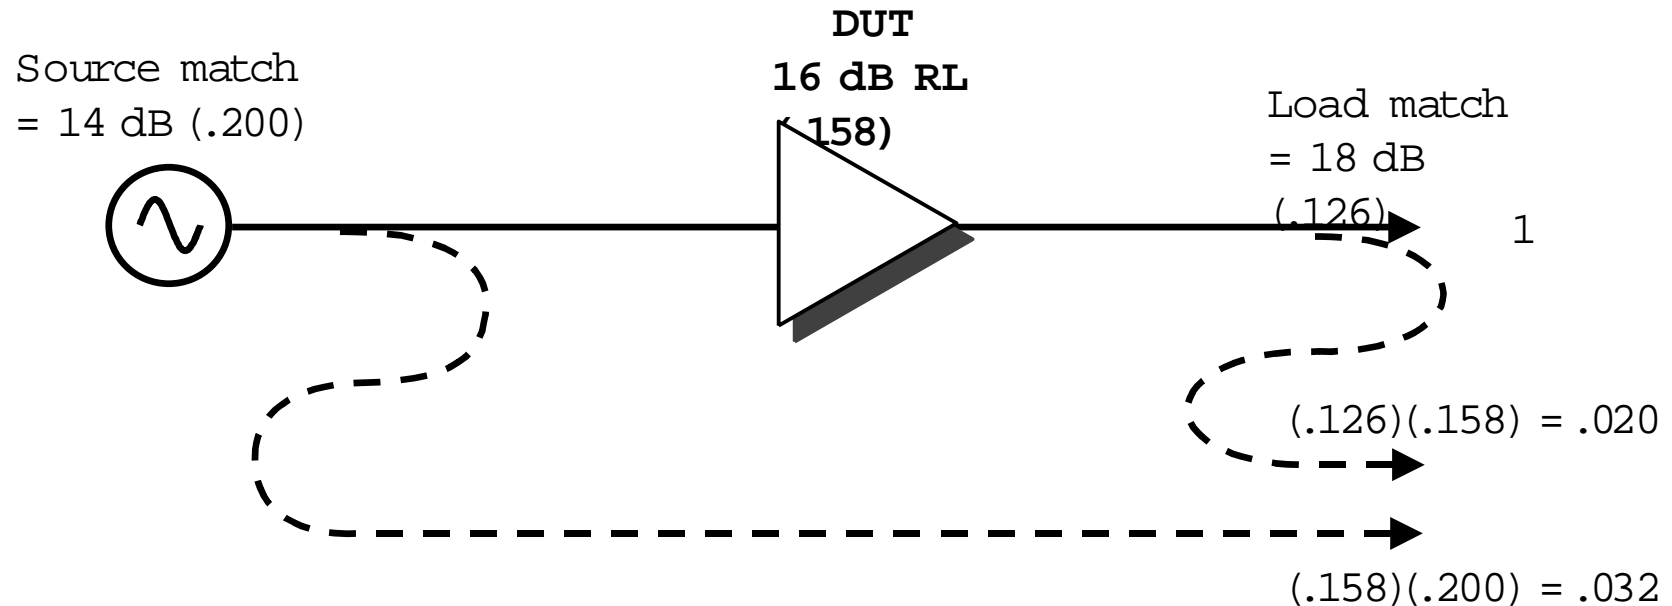


**Total measurement
uncertainty:**

$$+0.44 + 0.22 = + 0.66$$

dB

$$-0.46 - 0.22 = - 0.68$$

dB Network Analyzer Basics



Agilent Technologies

Measurement uncertainty

$$= 1 \pm (.020 + .032)$$

$$= 1 \pm .052$$

$$= + 0.44 \text{ dB}$$

$$- 0.46 \text{ dB}$$

Copyright
2000

Filter Measurements using the **Enhanced Response** Calibration

Effective source match =
35 dB!


Calibration Uncertainty

$$= (1 \pm \rho_S \rho_L)$$

$$= (1 \pm$$

$$(.0178)(.126)$$

$$= \pm .02 \text{ dB}$$

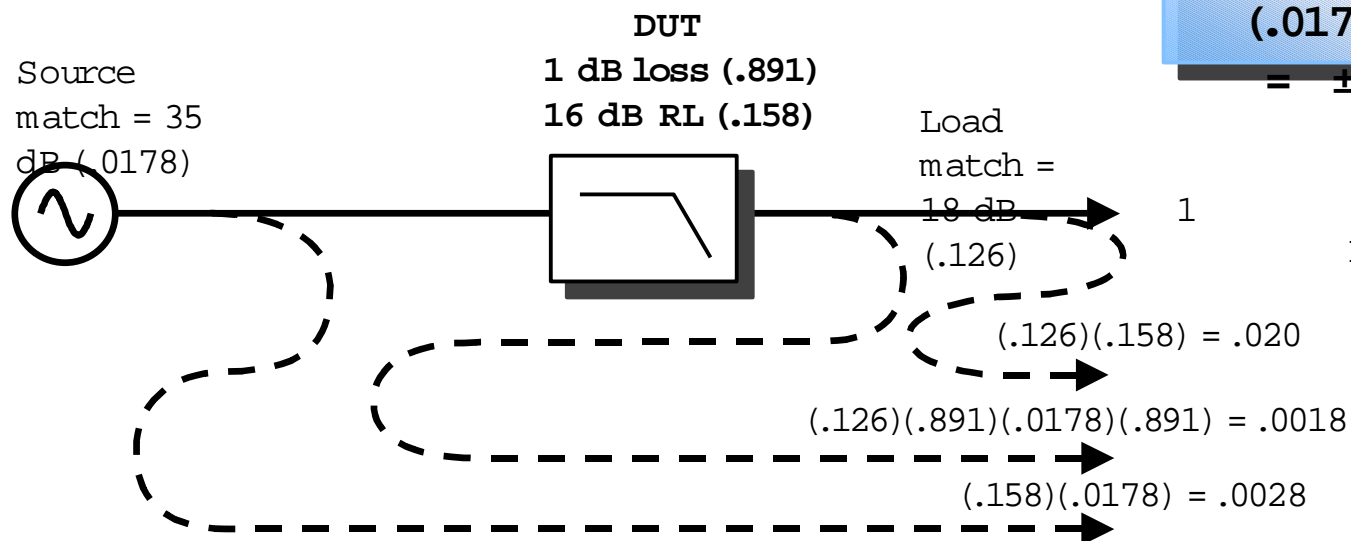

Measurement uncertainty

$$= 1 \pm (.020 + .0018 + .0028)$$

$$= 1 \pm .0246$$

$$= + 0.211 \text{ dB}$$

$$- 0.216 \text{ dB}$$

Total measurement
uncertainty:

$$0.22 + .02 = \pm 0.24 \text{ dB}$$



Using the *Enhanced Response* Calibration Plus an Attenuator

10 dB attenuator (.316)
 SWR = 1.05 (.024 linear or 32.4
 dB)
 Analyzer load match = 18 dB (.126)


Calibration Uncertainty

$$\pm 1 \pm \rho_S \rho_L$$

$$= (1 \pm$$

$$(.0178)(.0366)$$


$$= \pm .01 \text{ dB}$$

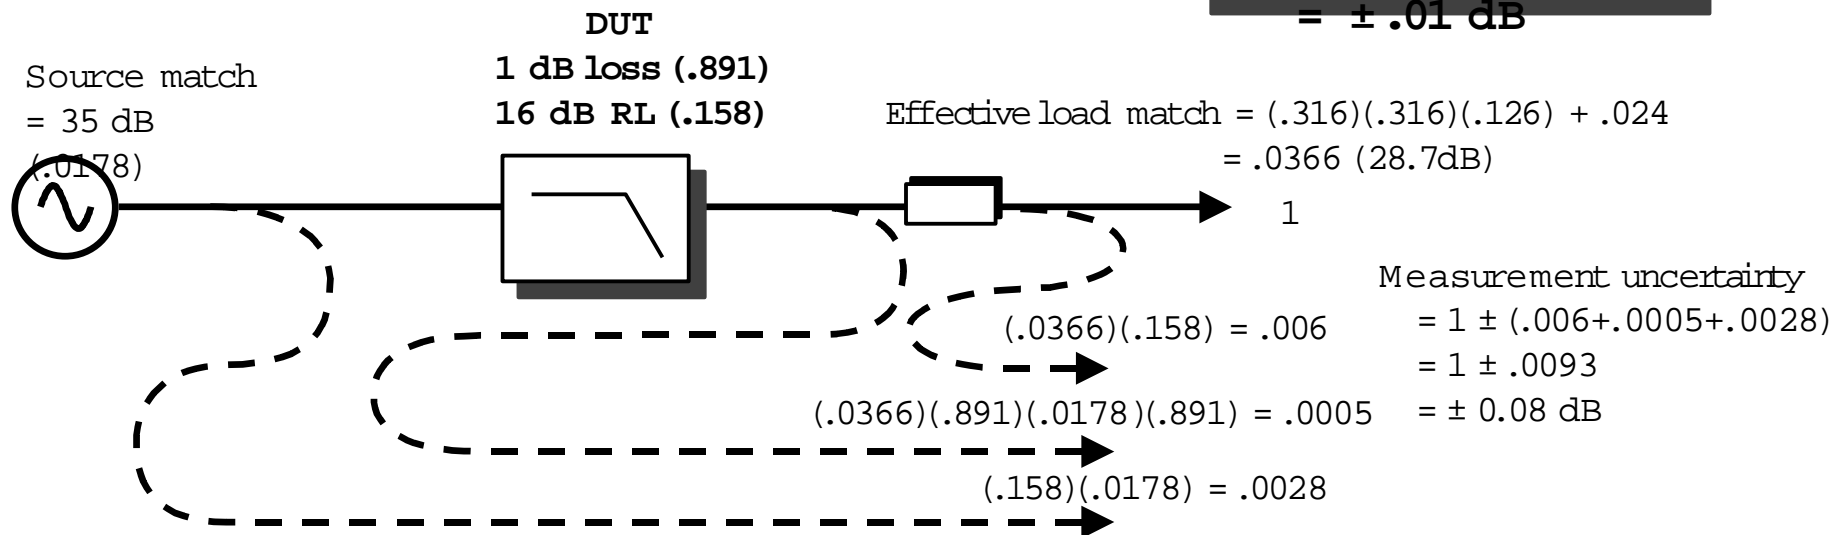

Total measurement uncertainty:

$$0.01 + .08 = \pm 0.09 \text{ dB}$$

Calculating Measurement Uncertainty After a Two-Port Calibration



DUT

1 dB loss (.891)

16 dB RL (.158)

Corrected error terms: (8753ES 1.3-3 GHz Type-N)

Directivity = 47

dB

Source match = 36 dB

Load match = 47

dB

Refl. tracking = .019

dB

Trans. tracking =

.026 dB

Isolation = 100 dB

Reflection uncertainty

$$\begin{aligned}
 S_{11m} &= S_{11a} \pm (E_D + S_{11a}^2 E_S + S_{21a} S_{12a} E_L + S_{11a} (1 - E_{RT})) \\
 &= 0.158 \pm (.0045 + 0.158^2 * .0158 + 0.891^2 * .0045 + 0.158 * .0022) \\
 &= 0.158 \pm .0088 = 16 \text{ dB } \mathbf{+0.53 \text{ dB}, -0.44 \text{ dB (worst-case)}}
 \end{aligned}$$


Transmission uncertainty

$$\begin{aligned}
 S_{21m} &= S_{21a} \pm S_{21a} (E_I / S_{21a} + S_{11a} E_S + S_{21a} S_{12a} E_S E_L + S_{22a} E_L + (1 - E_{TT})) \\
 &= 0.891 \pm 0.891 (10^{-6} / 0.891 + 0.158 * .0158 + 0.891^2 * .0158 * .0045 + 0.158 * .0045 + .003) \\
 &= 0.891 \pm .0056 = 1 \text{ dB } \mathbf{\pm 0.05 \text{ dB (worst-case)}}
 \end{aligned}$$



Response versus Two-Port Calibration


Measuring filter insertion loss

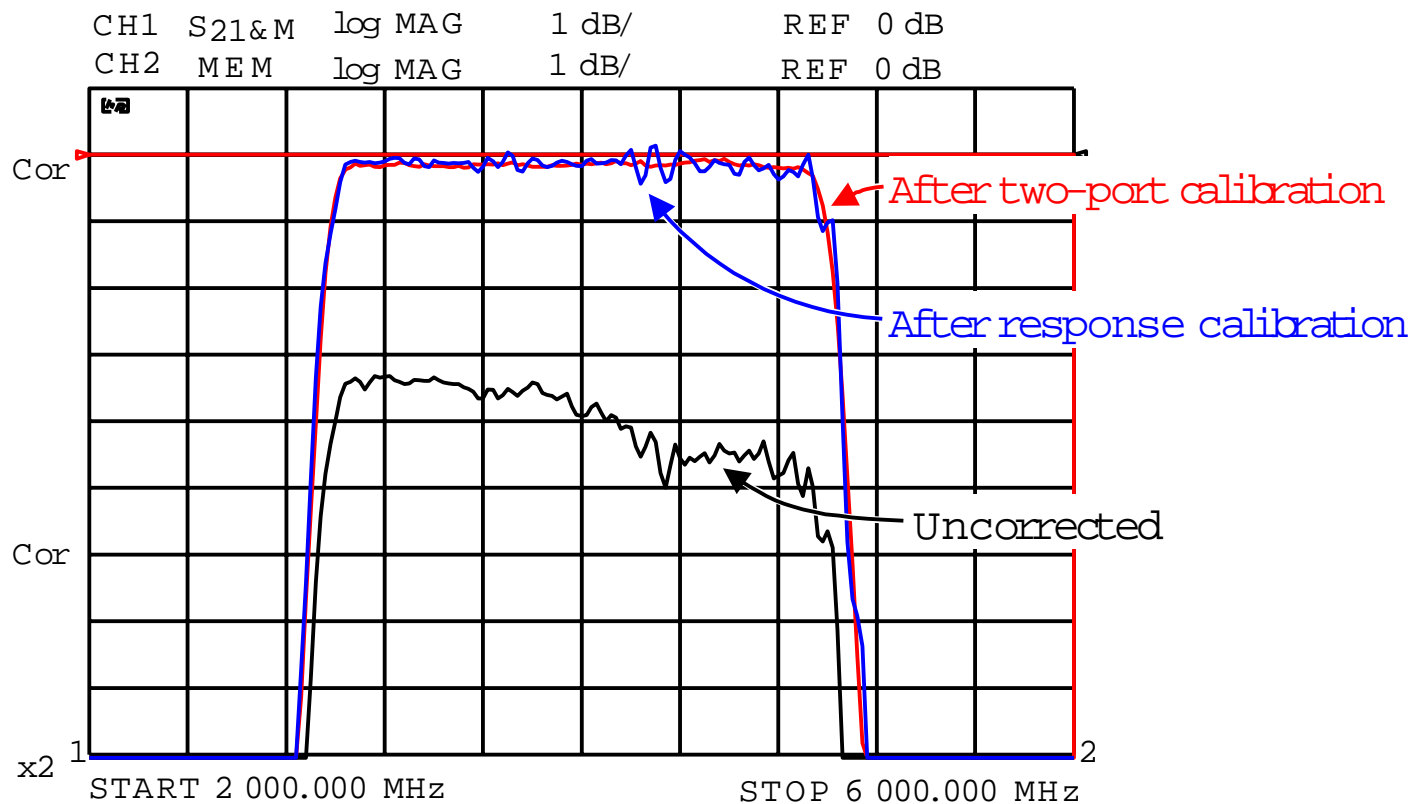

E Cal: Electronic Calibration (85060/90 series)

- . Variety of modules cover 30 kHz to 26.5 GHz
- . Six connector types available (50 Ω and 75 Ω)
- . Single-connection
 - reduces calibration time
 - makes calibrations easy to perform
 - minimizes wear on cables and standards
 - eliminates operator errors


~~Highly repeatable temperature~~
compensated terminations provide
excellent accuracy

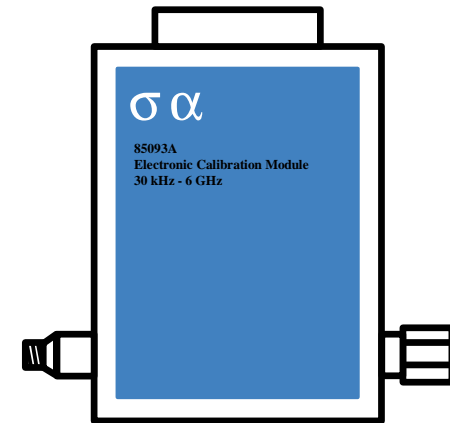

Microwave modules use a transmission line shunted by PIN-diode switches in various combinations




Adapter Considerations

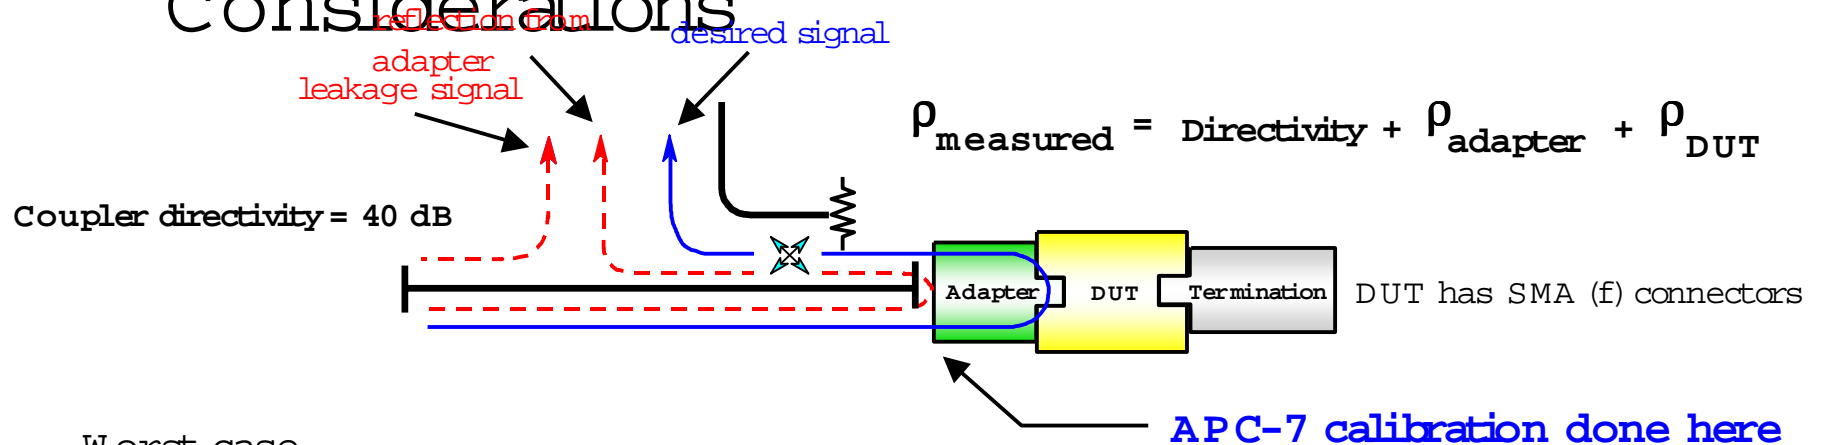

Worst-case
System Directivity


Adapting from APC-7 to SMA
(m)

28 dB




APC-7 to SMA (m)
SWR:1.06

17 dB



APC-7 to N (f) + N (m) to SMA (m)
SWR:1.05 SWR:1.25

14 dB



APC-7 to N (m) + N (f) to SMA (f) + SMA (m) to (m)
SWR:1.05 SWR:1.25 SWR:1.15



Calibrating Non-Insertable Devices

When doing a through cal, normally test ports mate directly

- cables can be connected directly without an adapter
- result is a zero-length through



What is an insertable device?

- has same type of connector, but different sex on each port
- has same type of sexless connector on each port (e.g. APC-7)




What is a non-insertable device?

- one that cannot be inserted in place of a zero-length through
- has same connectors on each port (type and sex)
- has different type of connector on each port (e.g., waveguide on one port, coaxial on the other)



What calibration holes do I have for non-

Swap Equal Adapters Method

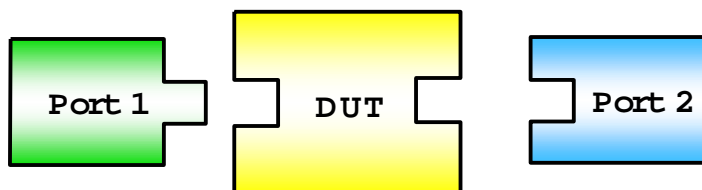


Accuracy depends on how well the adapters are matched - loss, electrical length, match and impedance should all be equal



1. Transmission cal using adapter A.



2. Reflection cal using adapter B.

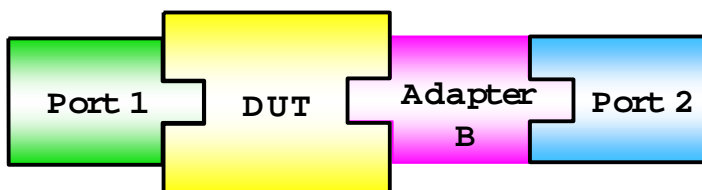


3. Measure DUT using adapter B.




Adapter Removal Calibration

- Calibration is very accurate and traceable
- In firmware of 8753, 8720 and 8510 series
- Also accomplished with ECal modules (85060)
- Uses adapter with same connectors as DUT
- Must specify electrical length of adapter to within 1/4 wavelength of highest frequency (to avoid phase ambiguity)

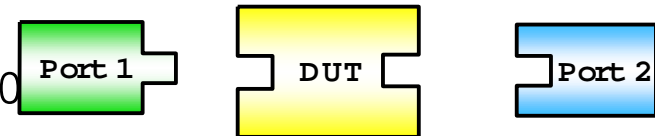

[CAL] [MORE] [MODIFY CAL SET]
[ADAPTER REMOVAL]



1. Perform 2-port cal with adapter on port 2. Save in cal set 1.
2. Perform 2-port cal with adapter on port 1. Save in cal set 2.
3. Use ADAPTER REMOVAL to generate new cal set.
4. Measure DUT without cal adapter.




Thru-Reflect-Line (TRL) Calibration

We know about Short-Open-Load-Thru (SOLT) calibration...


What is TRL?

- A two-port calibration technique
- Good for noncoaxial environments (waveguide, fixtures, wafer probing)
- Uses the same 12-term error model as the more common SOLT cal
- Uses practical calibration standards that are easily fabricated and characterized
- Two variations: TRL (requires 4 receiver measurements) and TRL* (only three receivers needed)
- Other variations: Line-Reflect-Match (LRM), Thru-Reflect-Match (TRM), plus many others



*TRL was developed for **non-coaxial microwave** measurements*

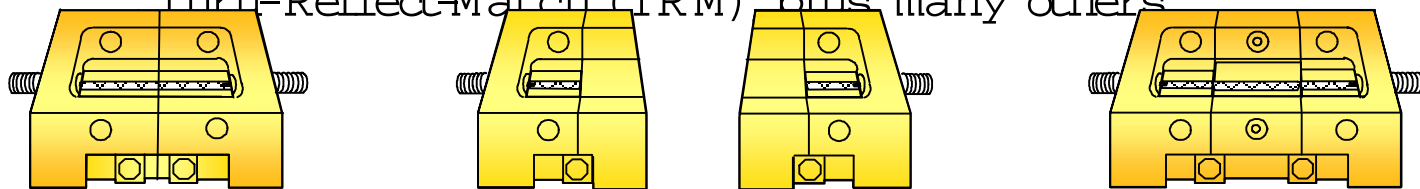

Agenda

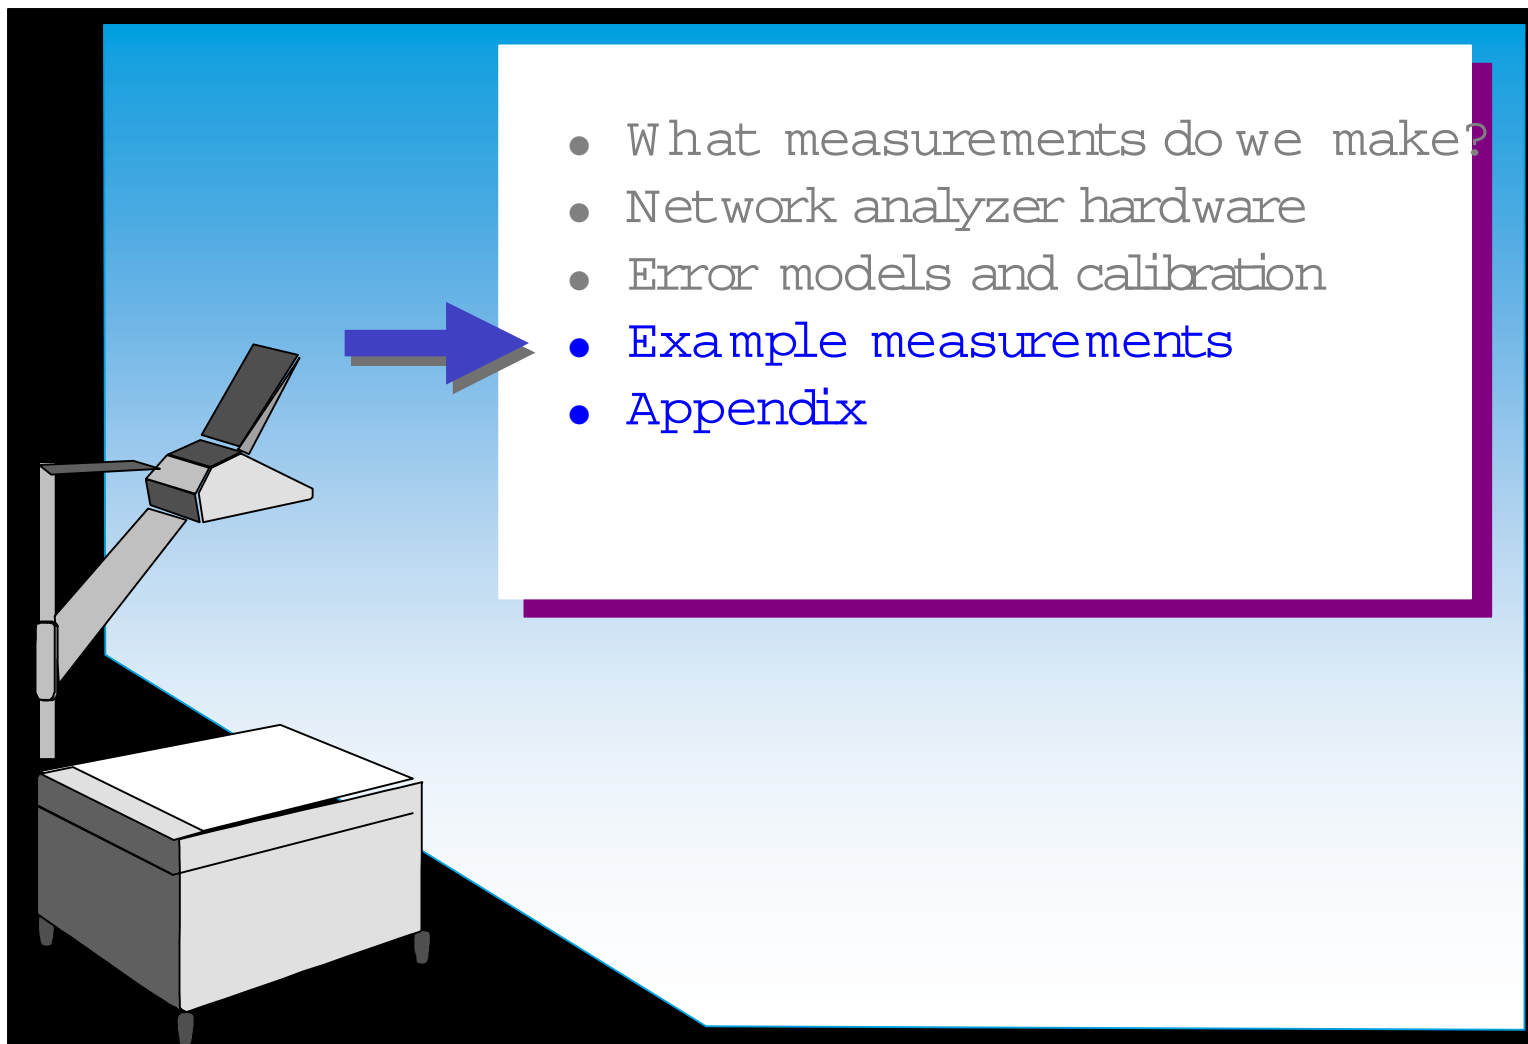


Frequency Sweep – Filter Test

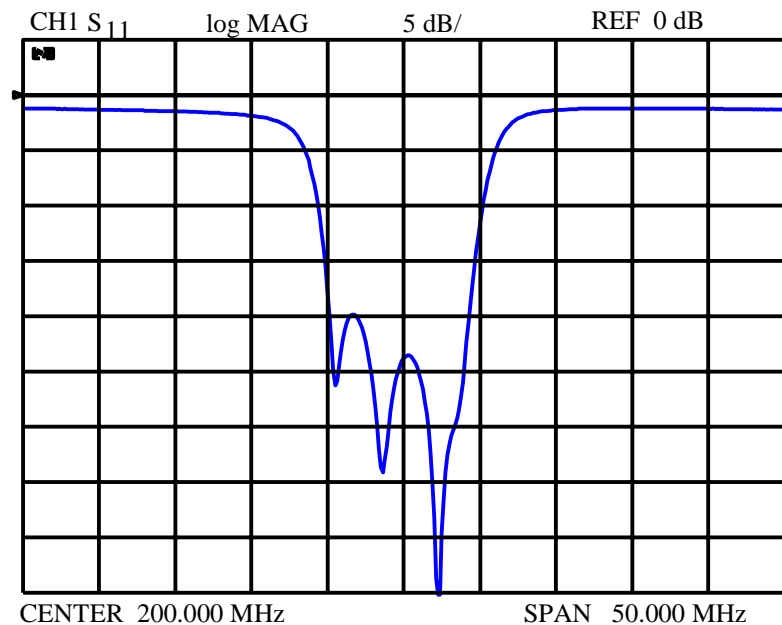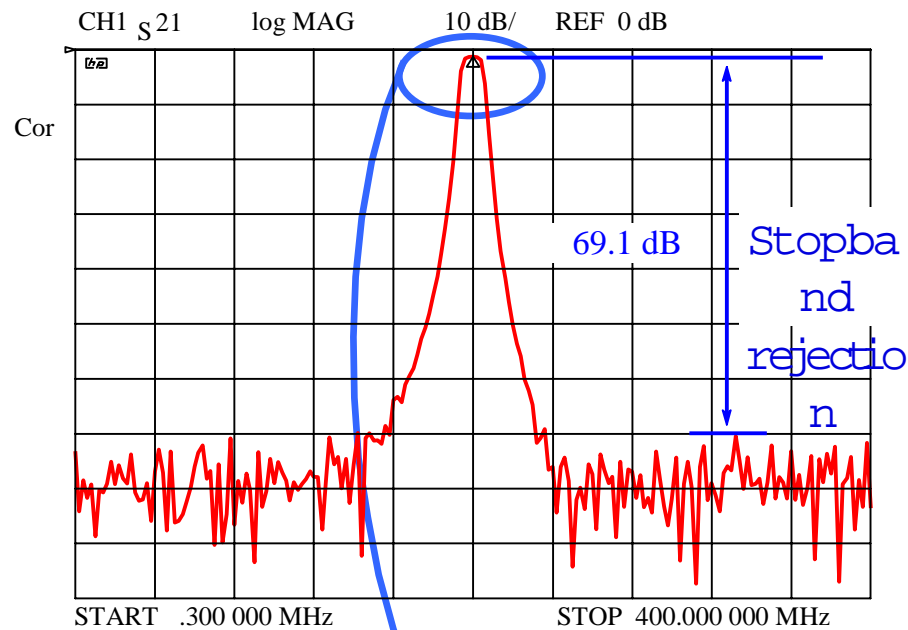


Return loss


Insertion loss

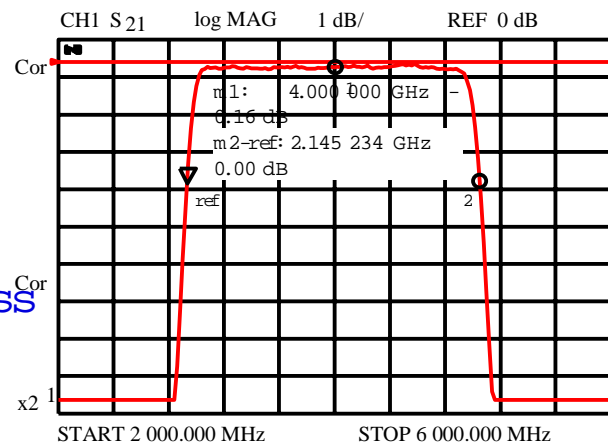

Optimize Filter Measurements with Swept-List Mode

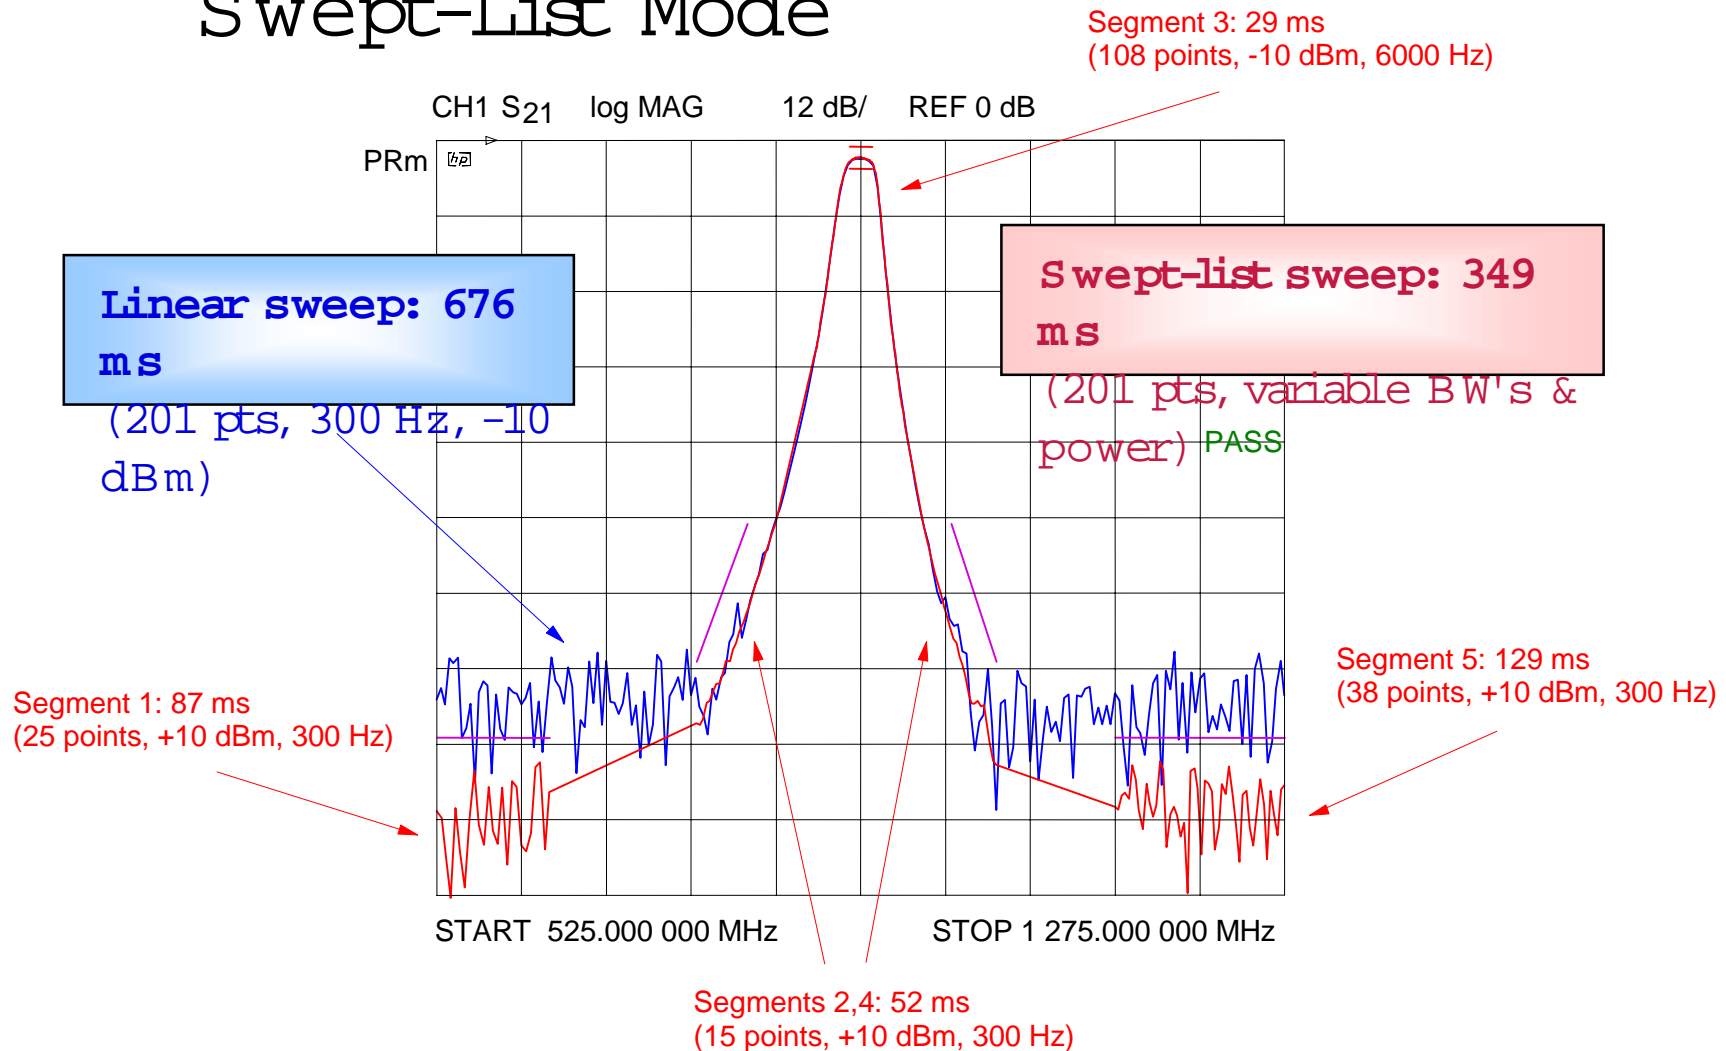


Power Sweeps - Compression

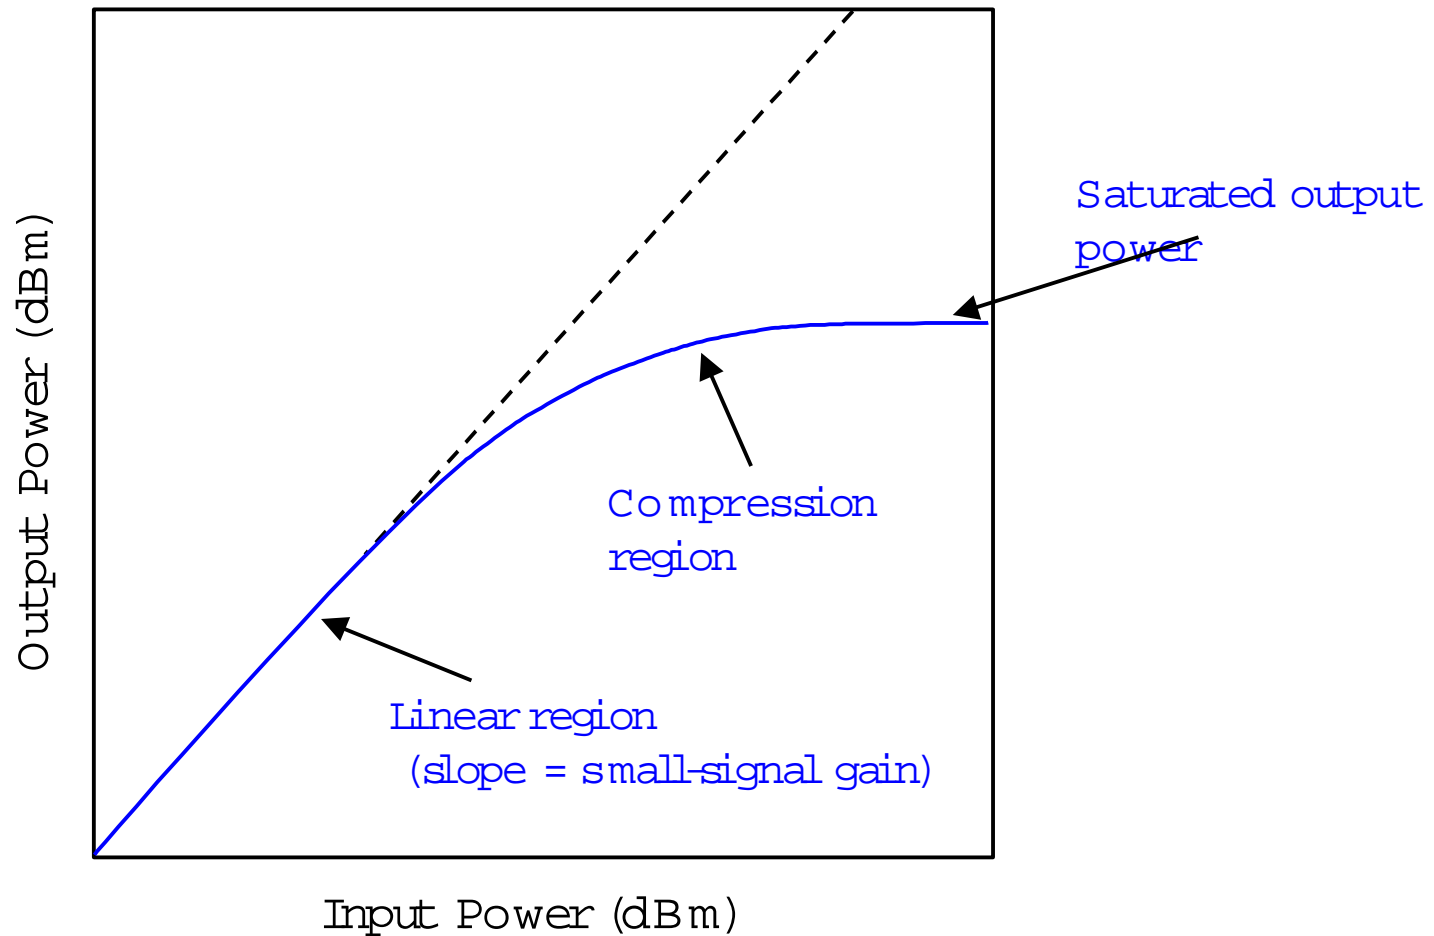

Power Sweep - Gain Compression

CH1 S21 log MAG 1 dB/ REF 32 dB 30.991 dB
12.3 dBm




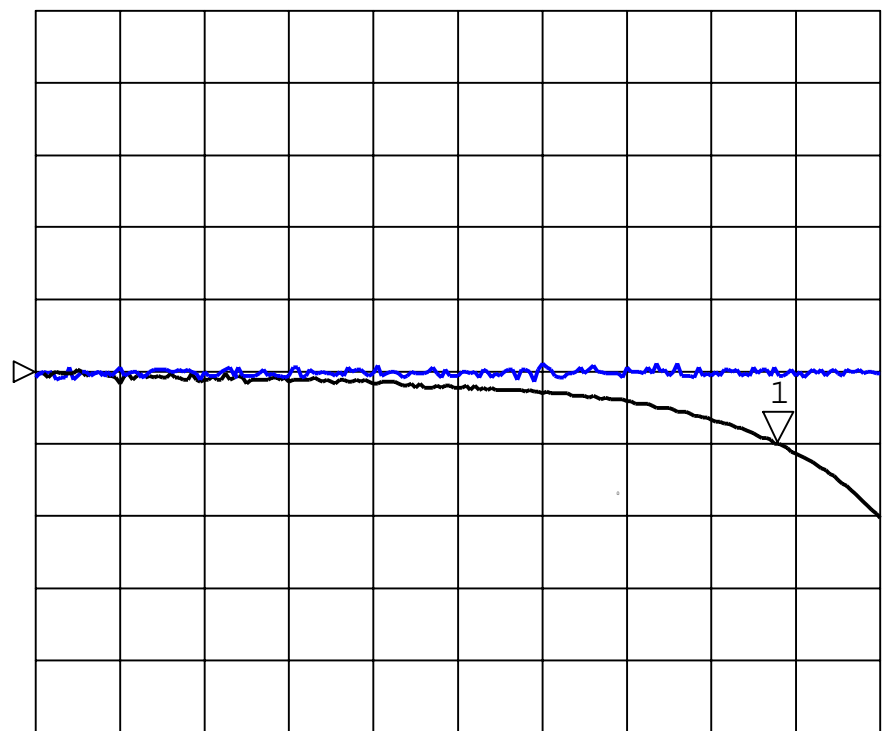


START -10 dBm CW 902.7 MHz STOP 15 dBm

**1 dB
compression:**
input power
resulting in 1 dB
drop in gain


AM to PM Conversion

Measure of phase deviation caused by amplitude variations

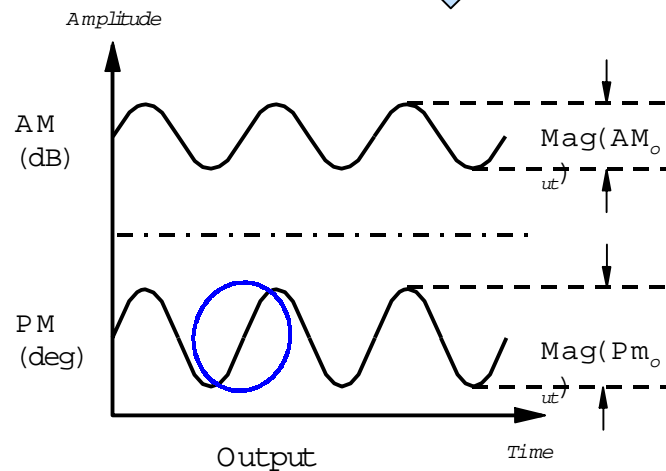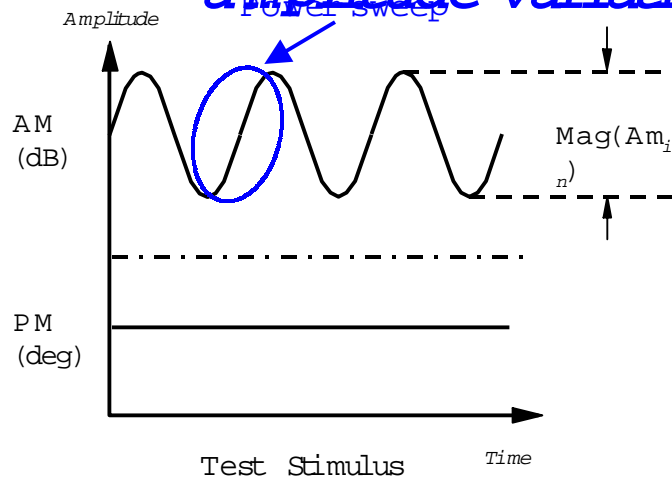

- AM can be undesired: supply ripple, fading, thermal
- AM can be desired: modulation (e.g. QAM)

$$\text{AM - PM Conversion} = \frac{\text{Mag(Pm}_{out})}{\text{Mag(Am}_{in})} \text{ (deg/dB)}$$

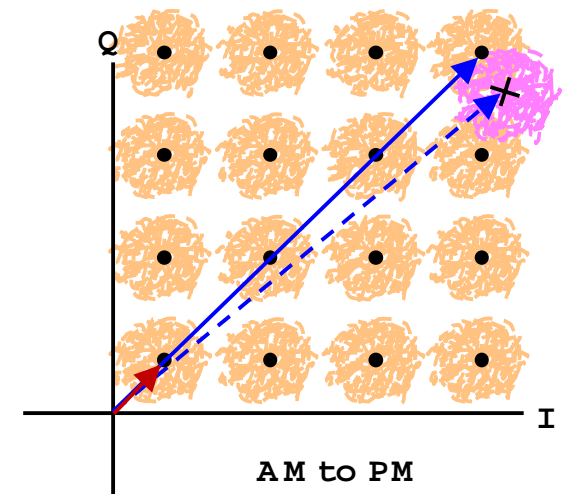


AM to PM conversion can cause bit errors

Copyright
2000




Measuring AM to PM Conversion

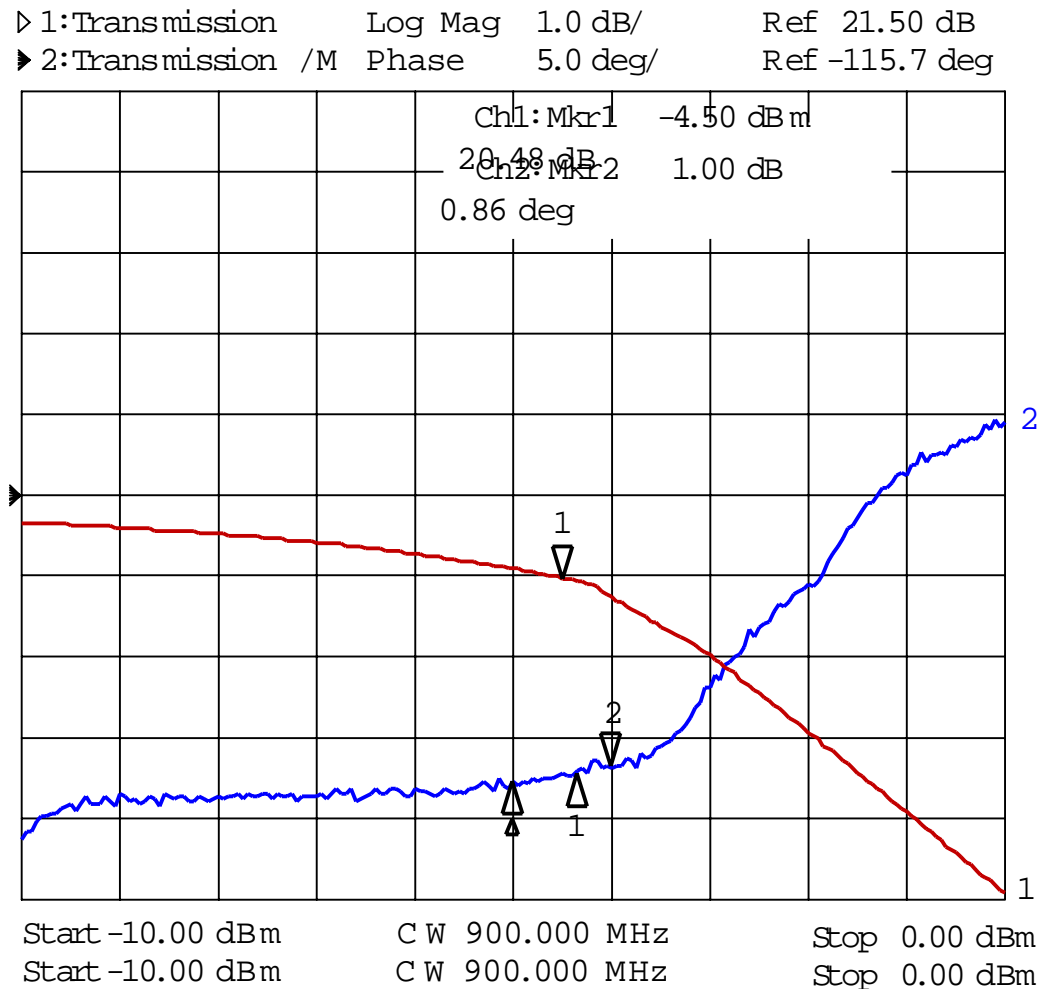

- Use transmission setup with a power sweep
- Display phase of S21
- AM - PM = 0.86 deg/dB



Agenda

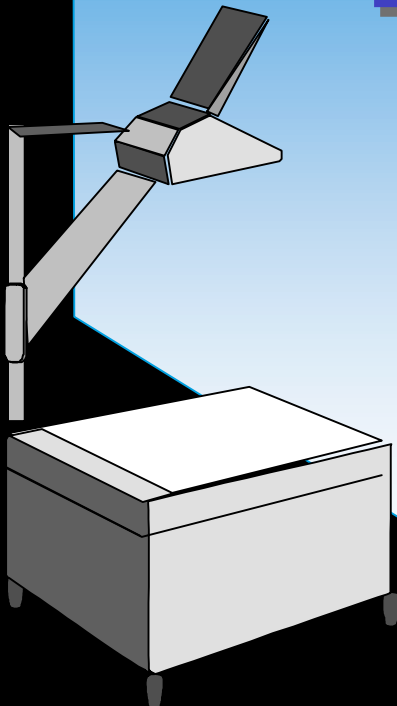


- What measurements do we make?
- Network analyzer hardware
- Error models and calibration
- Example measurements
- **Appendix**
 - Advanced Topics
 - time domain
 - frequency-translating devices
 - high-power amplifiers
 - extended dynamic range
 - multiport devices
 - in-fixture measurements
 - crystal resonators
 - balanced/differential
 - Inside the network analyzer
 - Challenge quiz!





Time-Domain Reflectometry (TDR)

- What is TDR?
 - time-domain reflectometry
 - analyze impedance versus time
 - distinguish between inductive and capacitive transitions
- With gating:
 - analyze transitions
 - analyzer standards

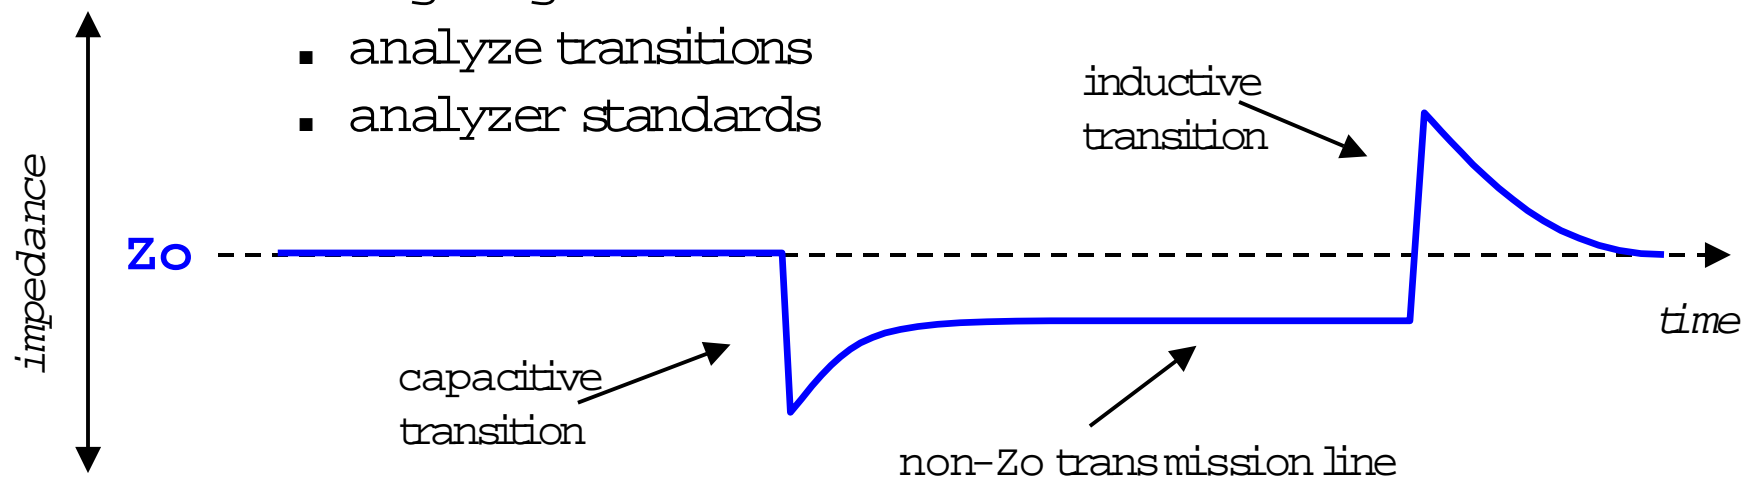



TDR Basics Using a Network Analyzer

- start with broadband frequency sweep (often requires microwave VN)
- use inverse-Fourier transform to compute time-domain
- resolution inversely proportionate to frequency span

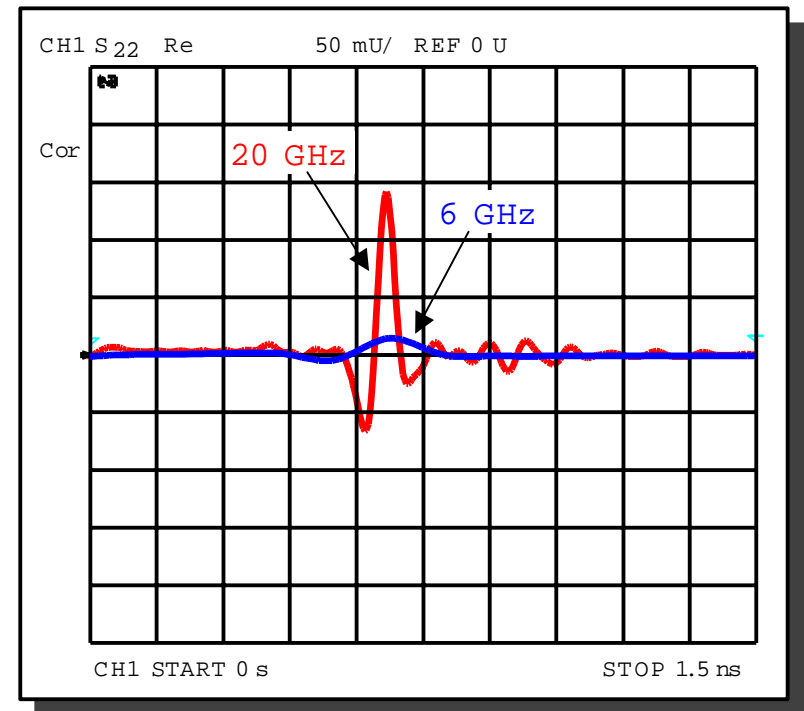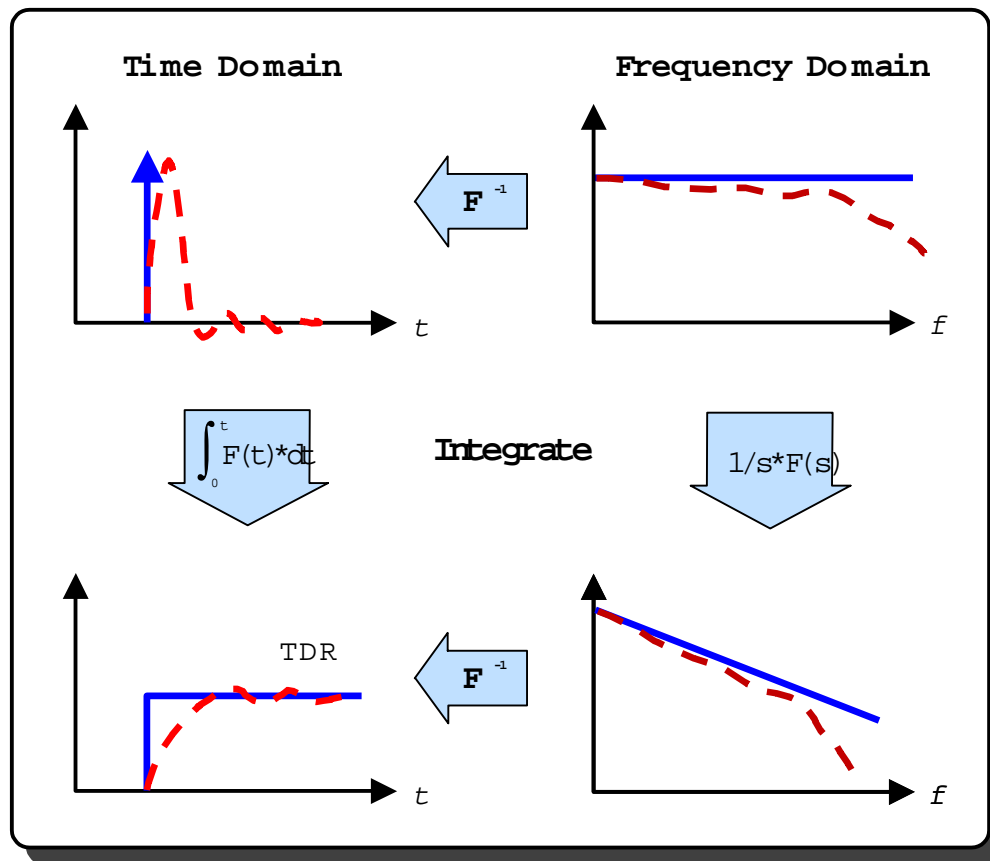

Time-Domain Gating

- TDR and gating can **remove** undesired reflections (a form of error **correction**)
- Only useful for **broadband** devices (a load or thru for example)
- Define **gate** to only include DUT
- Use two-port calibration


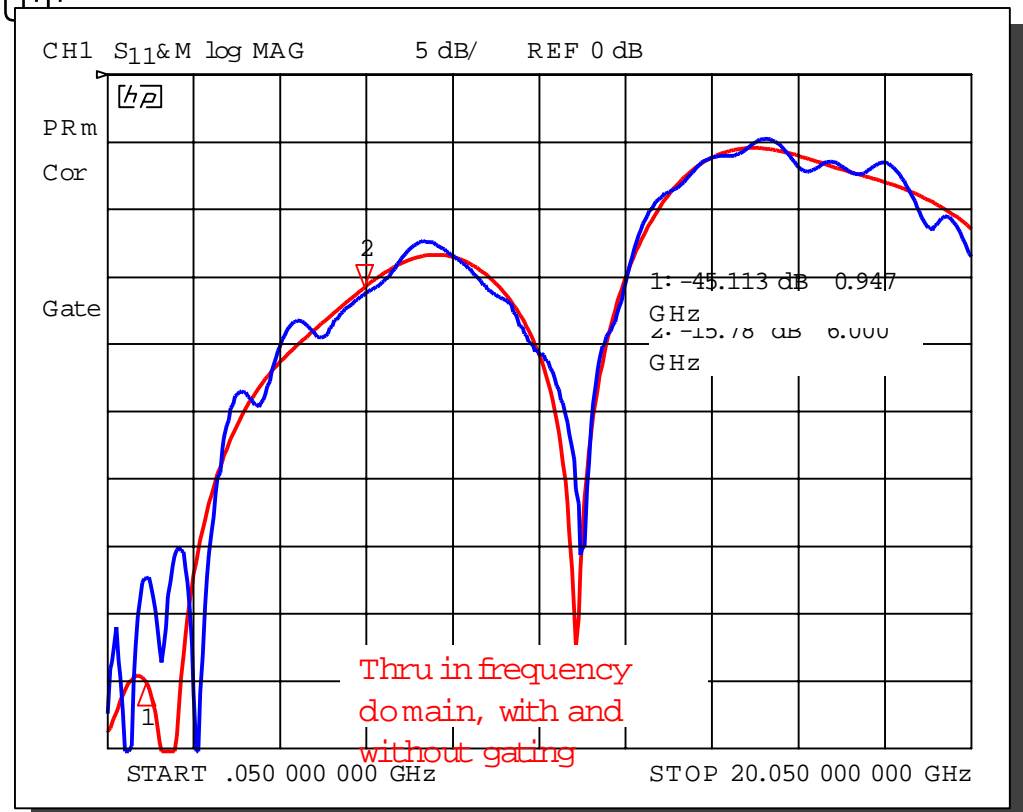
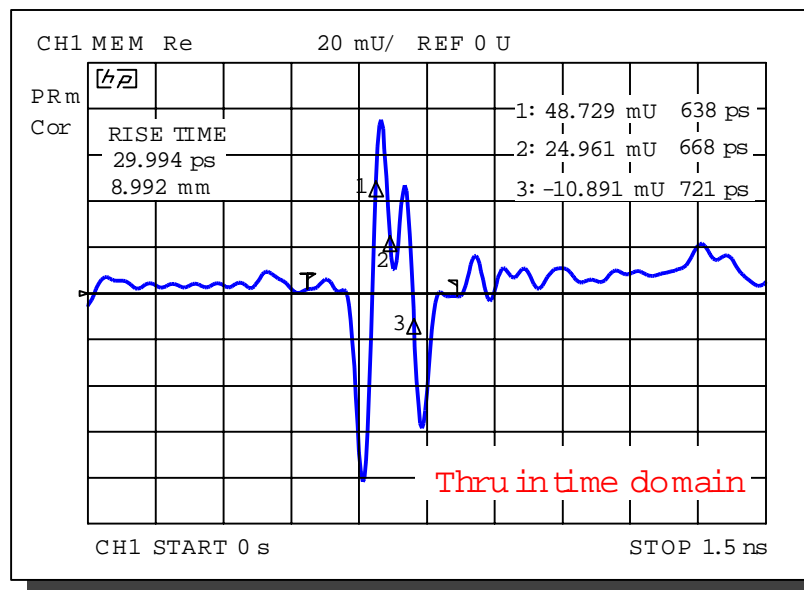


Ten Steps for Performing TDR


1. Set up desired frequency range (need wide span for good spatial resolution)
2. Under SYSTEM, transform menu, press "set freq low pass"
3. Perform one- or two-port calibration
4. Select S11 measurement *
5. Turn on transform (low pass step) *
6. Set format to real *
7. Adjust transform window to trade off rise time with ringing and overshoot *
8. Adjust start and stop times if desired
9. For gating:
 - set start and stop frequencies for gate
 - turn gating on *
 - adjust gate shape to trade off resolution with ripple *
10. To display gated response in frequency domain
 - * ~~if using transform off (leave gating on)~~ parameters must be set independently for second channel *
 - * change format to log magnitude *



Time-Domain Transmission

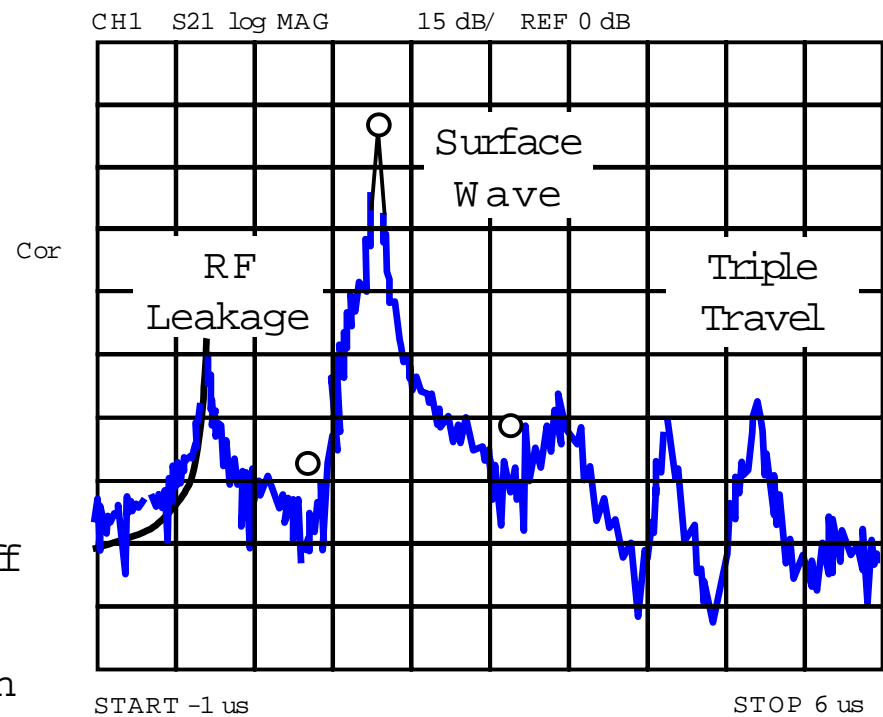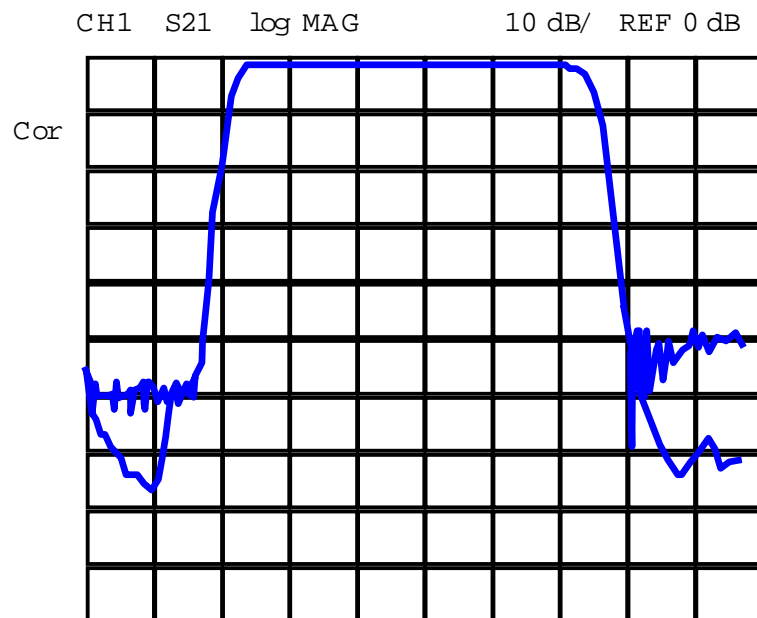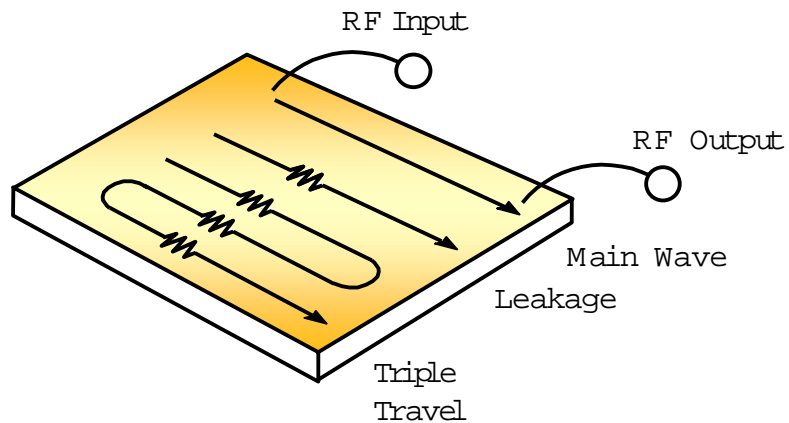


Time-Domain Filter Tuning

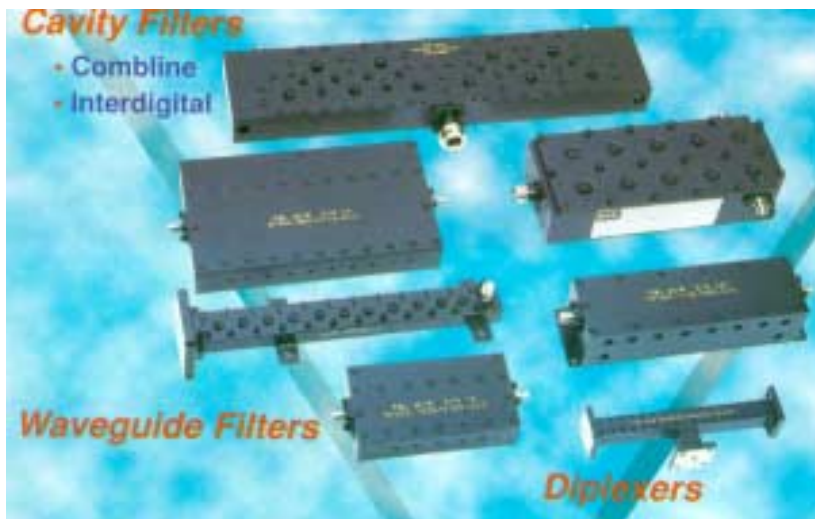

- Deterministic method used for tuning cavity-resonator filters
- Traditional frequency-domain tuning is very difficult:
 - lots of training needed
 - may take 20 to 90 minutes to tune a single filter
- Need VNA with fast sweep speeds and fast time-domain processing




Filter Reflection in Time Domain

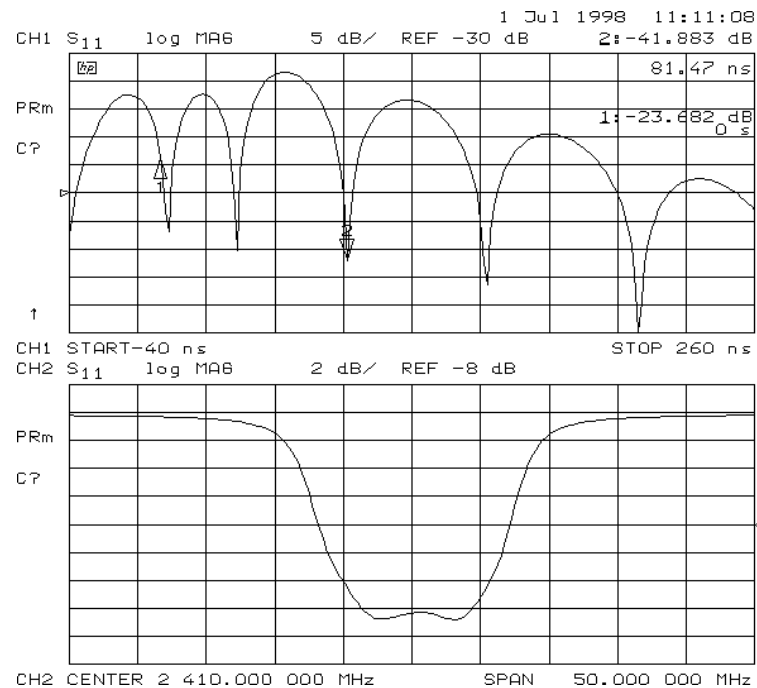

- Set analyzer's center frequency
= center frequency of the filter
- Measure S_{11} or S_{22} in the time domain
- Nulls in the time-domain response correspond to individual resonators in filter



Tuning Resonator #3

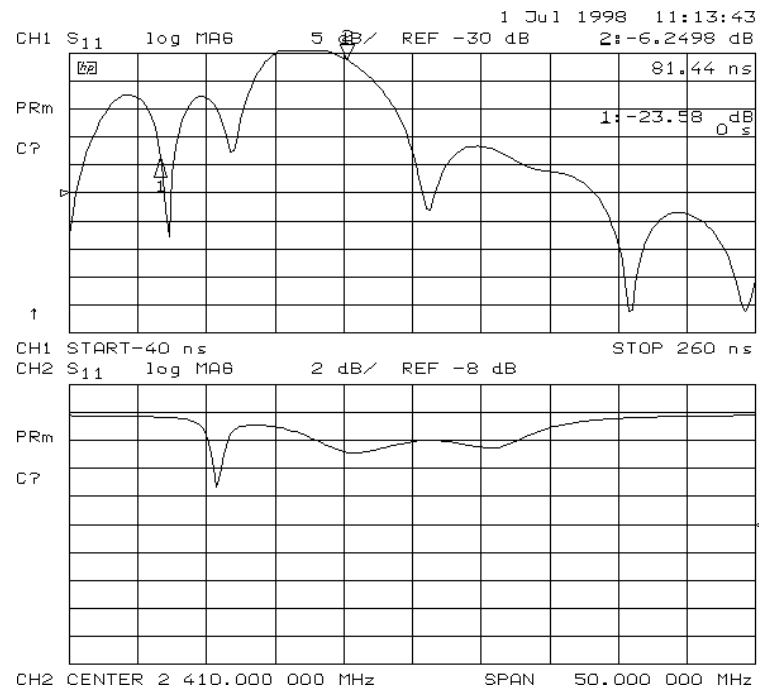


- Easier to identify mistuned resonator in time-domain: null #3 is missing
- Hard to tell which resonator is mistuned from frequency-domain response
- Adjust resonators by minimizing null
- Adjust coupling apertures using the peaks in-between the dips




Frequency-Translating Devices




Medium-dynamic range
measurements (25 dB)

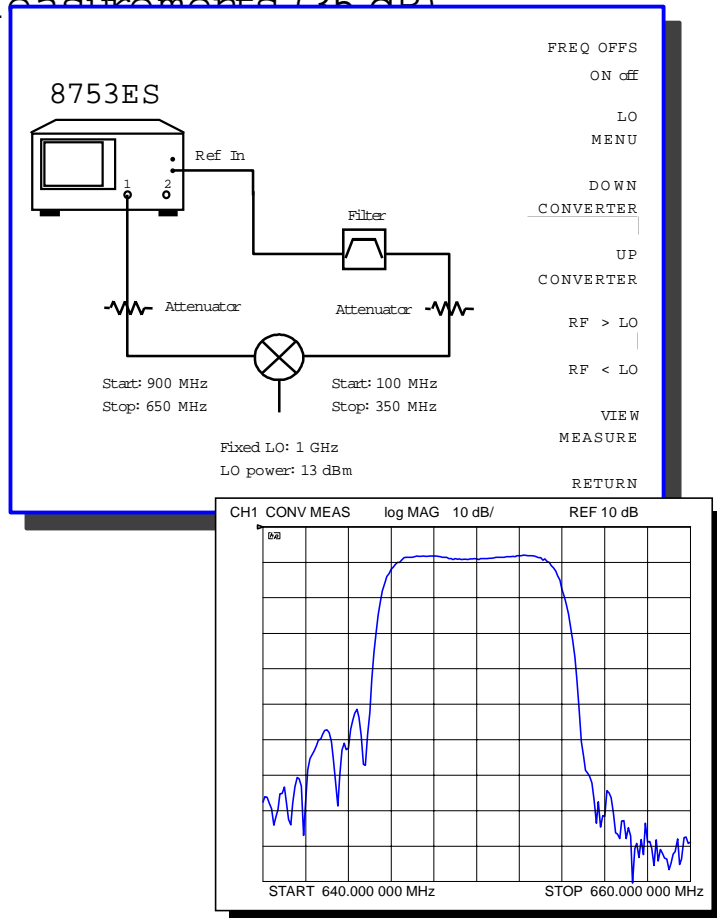

High-dynamic range measurements
(100 dB)

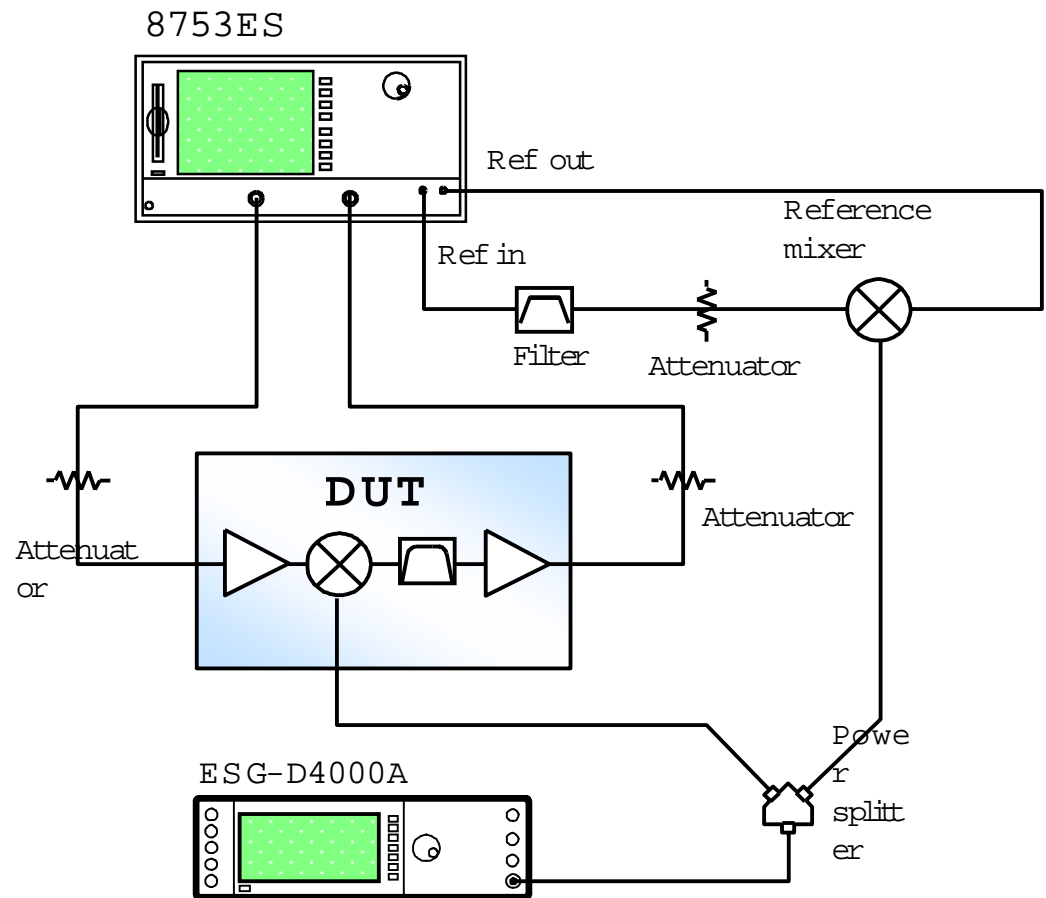


High-Power Amplifiers

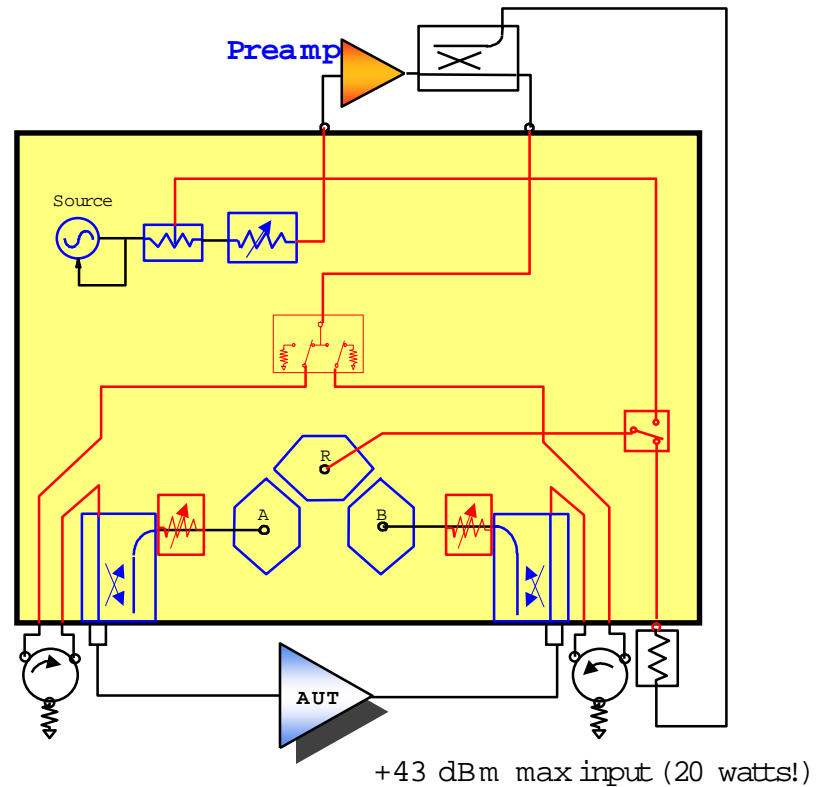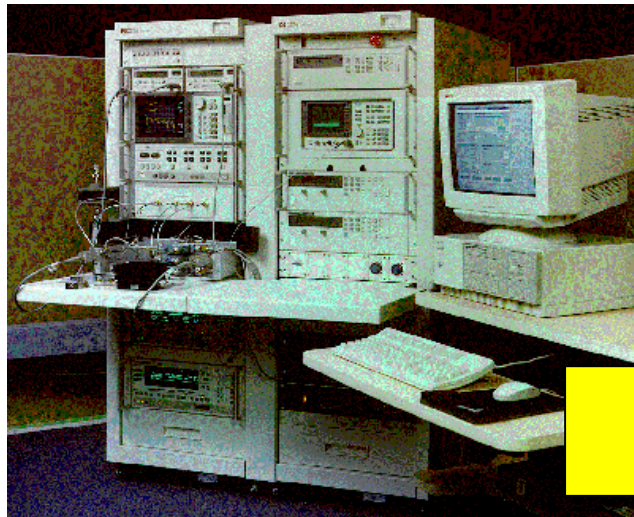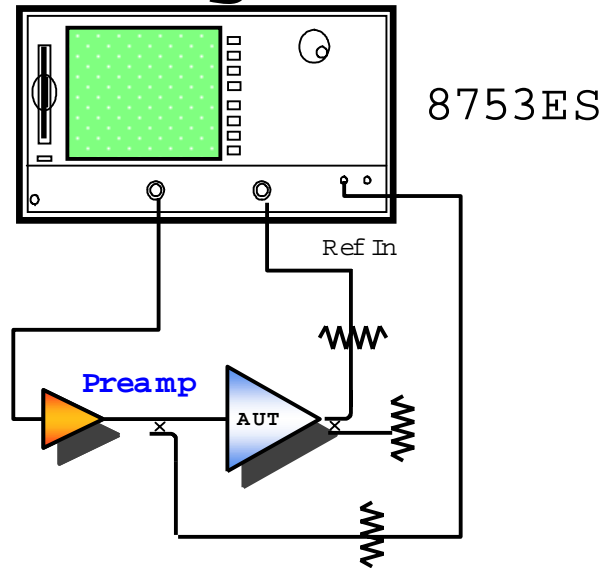

85118A High-Power
Amplifier Test System




High-Dynamic Range Measurements

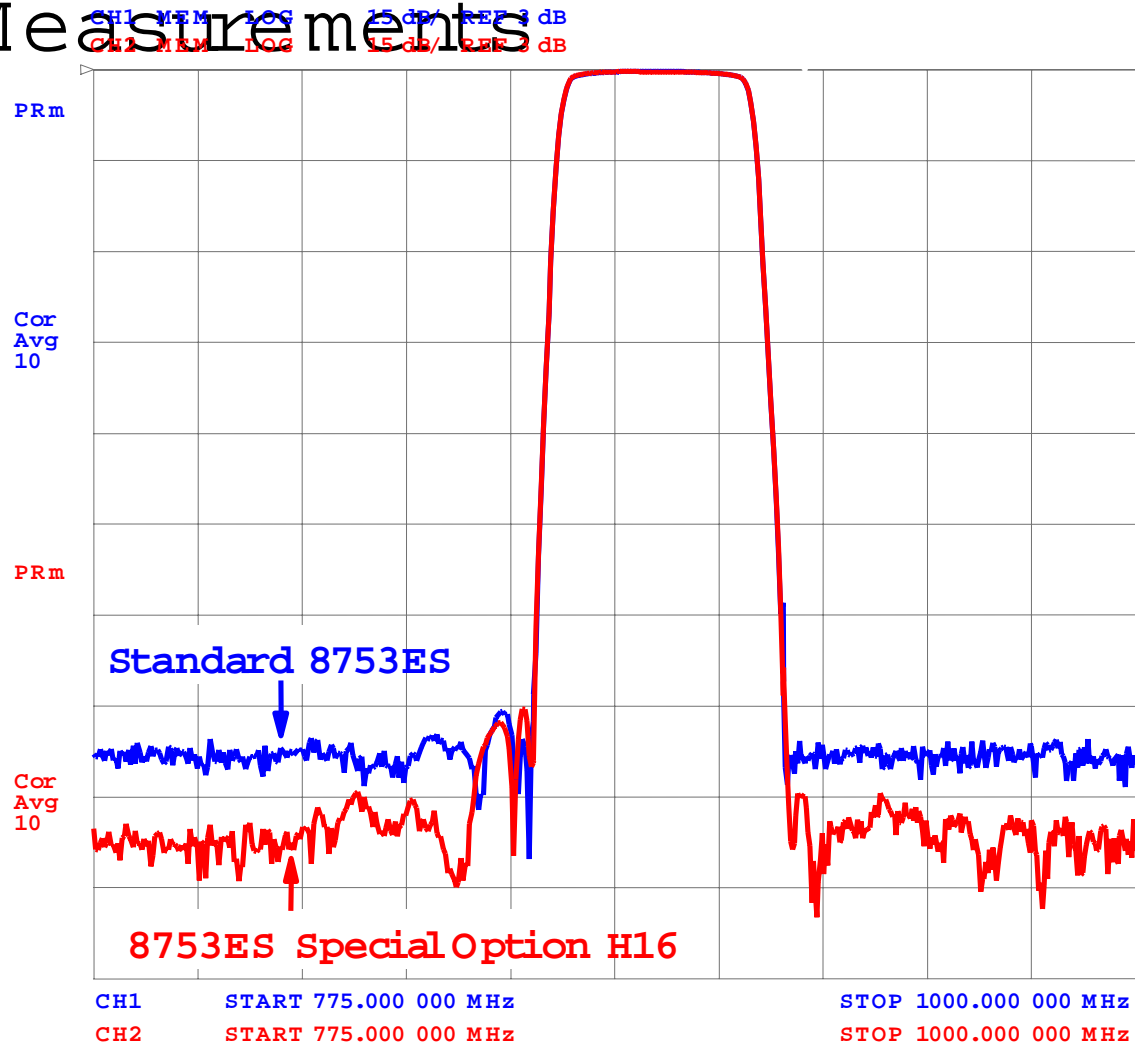

Multiport Device Test



8753 H39

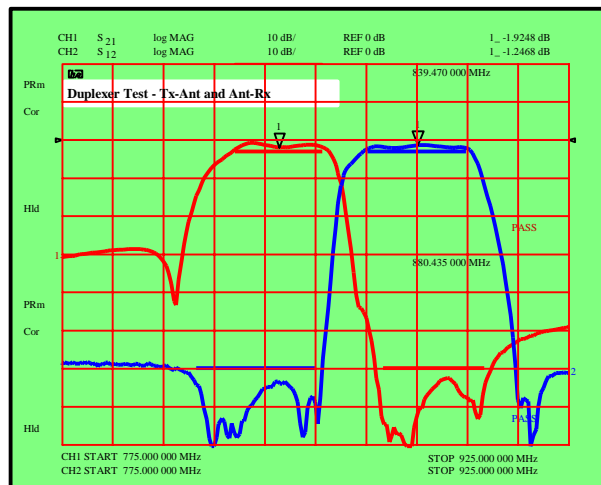

Multiport analyzers and test sets:


- improve **throughput** by reducing the number of connections to DUTs with more than two ports
- allow **simultaneous** viewing of two paths (good for tuning duplexers)
- include **mechanical** or **solid-state** switches, 50 or 75 ohms
- degrade raw performance so **calibration** is a **must** (use two-port cals whenever possible)
- Agilent offers a variety of standard and custom multiport analyzers and test sets



87050E/87075C Standard Multiport Test Sets



Once a month:
perform a **Test Set Cal** with
external standards to remove
systematic errors in the
~~analyzer, test set, cables, and~~
fixture

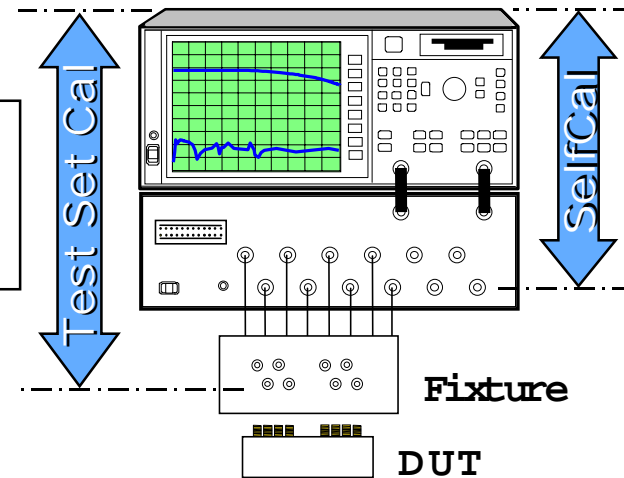


Once an hour:
automatically perform a
SelfCal using internal
standards to remove
systematic errors in the
~~analyzer and test set~~

- For use with 8712E family
- 50 Ω : 3 MHz to 2.2 GHz , 4, 8, or 12 ports
- 75 Ω : 3 MHz to 1.3 GHz , 6 or 12 ports
- Test Set Cal and SelfCal dramatically improve calibration times
- Systems offer fully-specified performance at test ports




Test Set Cal Eliminates Redundant Connections of Calibration Standards

Reflection Connections

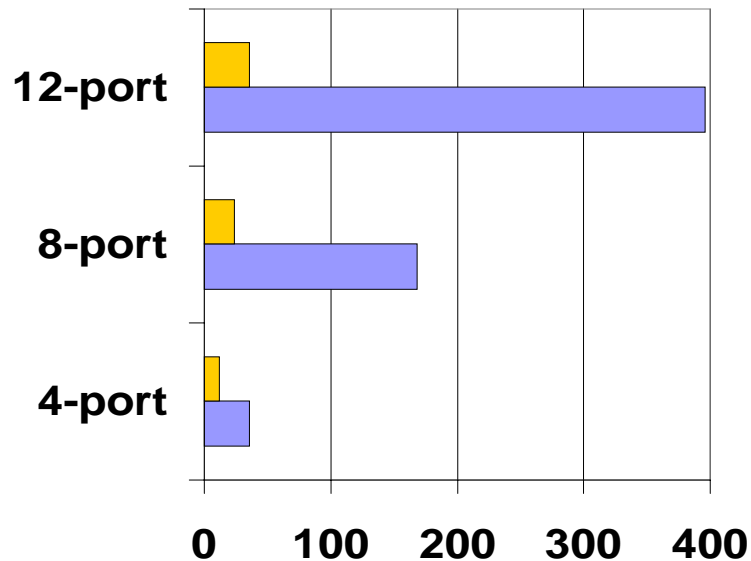

Through Connections

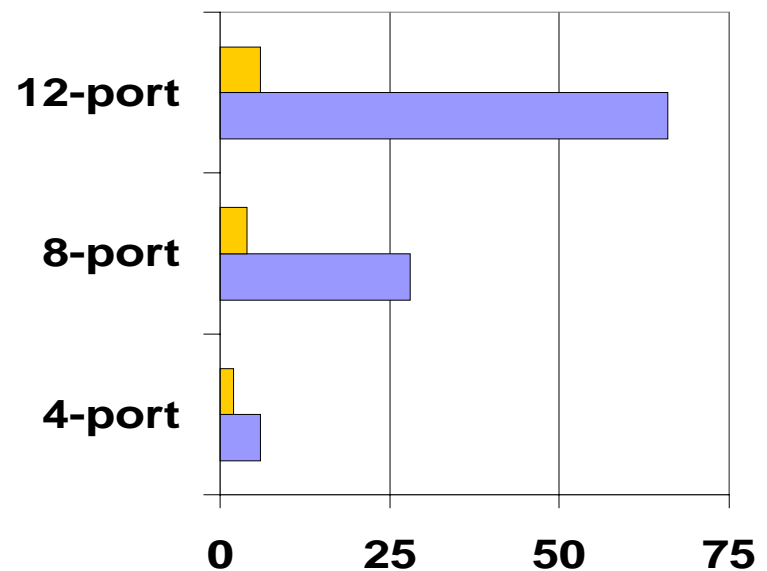

Test Set Cal




Traditional VNA Calibration



Agilent Technologies


In-Fixture Measurements

Measurement problem: coaxial calibration plane is not the same as the in-fixture measurement plane

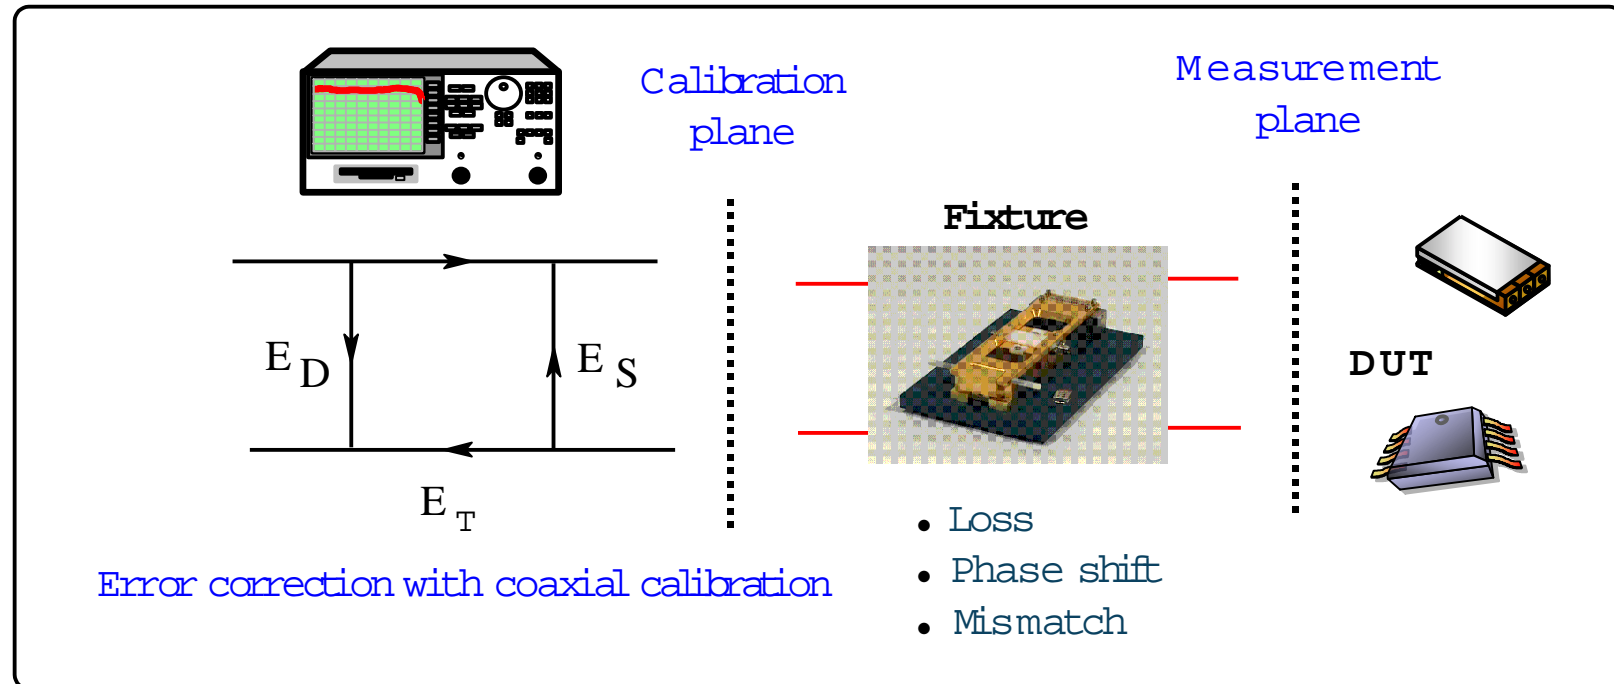

Characterizing Crystal Resonators/Filters

E5100A/B Network Analyzer

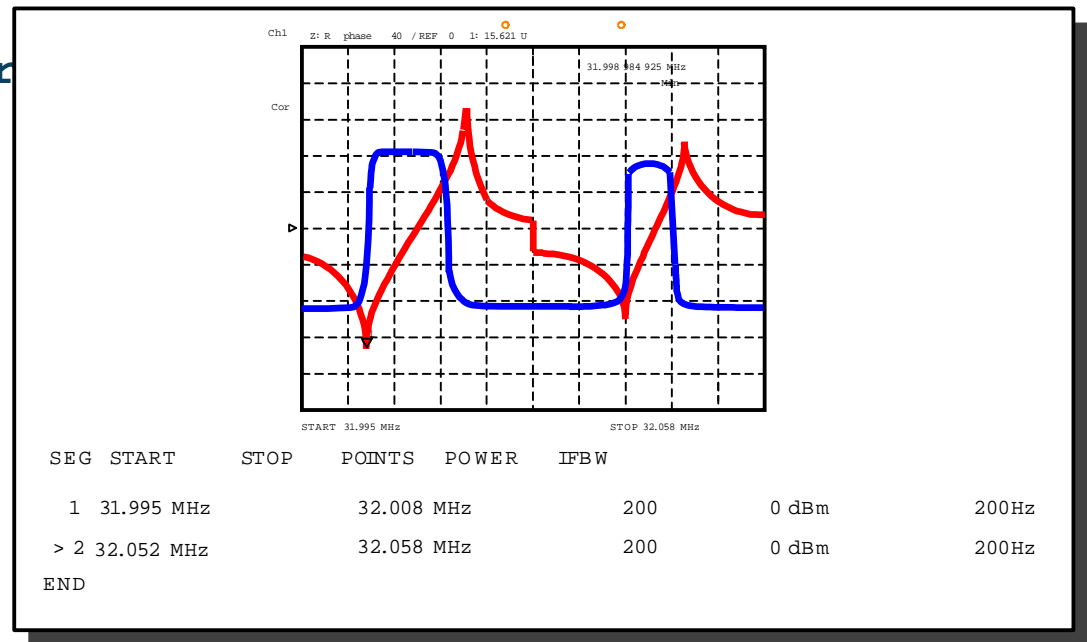


Example of crystal resonator
measurement



Balanced-Device Measurements

- **ATN-4000 series (4-port test set + software)**
- measure tough singled-ended devices like **couplers**
- measure **fully-balanced or single-ended-to-balanced** DUTs
- characterize mode conversions (e.g. common-to-differential)
- incorporates **4-port error correction** for exceptional accuracy
- works with 8753ES and 8720ES analyzers
- more info at www.atnmicrowave.com

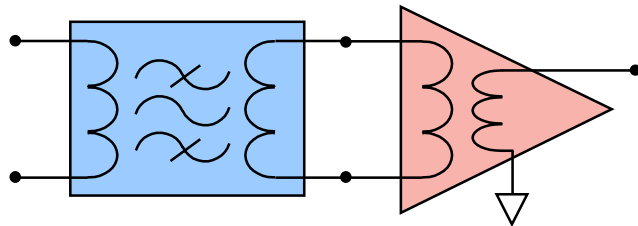


Traditional Scalar Analyzer




processor/display

source

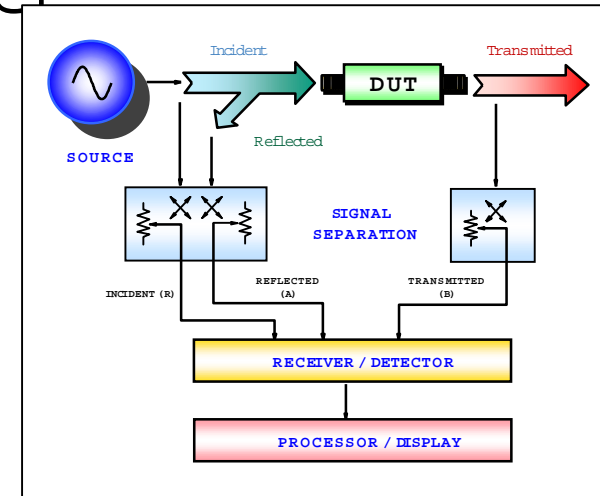


Example: **8757D/E**

- requires external detectors, couplers, bridges, splitters
- good for low-cost microwave scalar applications

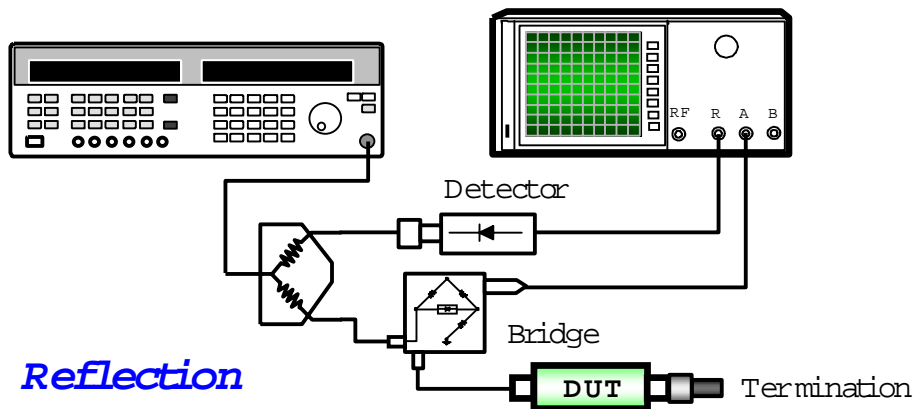

Reflection

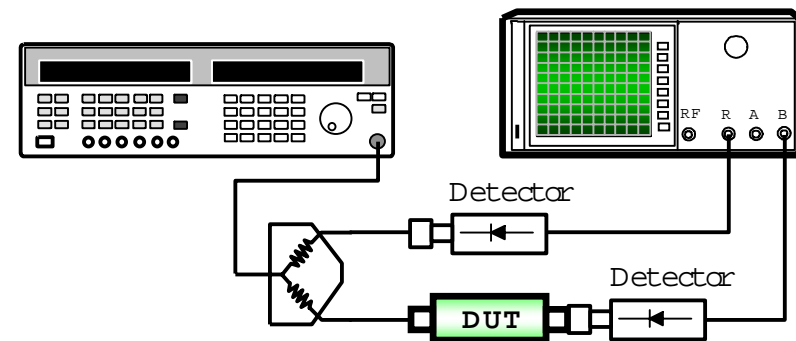

Transmission




Directional Coupler *Directivity*


$$\text{Directivity} = \frac{\text{Coupling Factor}_{(\text{fwd})} \times \text{Loss}}{\text{Isolation}_{(\text{rev})}}$$

$$\text{Directivity (dB)} = \text{Isolation (dB)} - \text{Coupling Factor (dB)} - \text{Loss (dB)}$$


Examples:

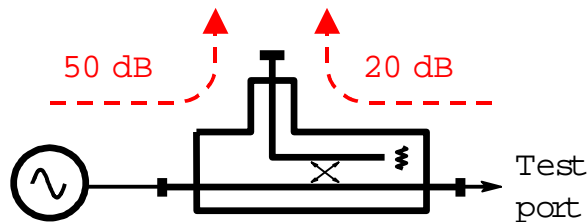

$$\text{Directivity} = 50 \text{ dB} - 20 \text{ dB} = 30 \text{ dB}$$

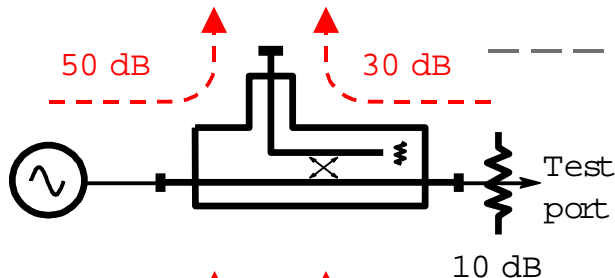



$$\text{Directivity} = 50 \text{ dB} - 30 \text{ dB} - 10 \text{ dB} = 10 \text{ dB}$$

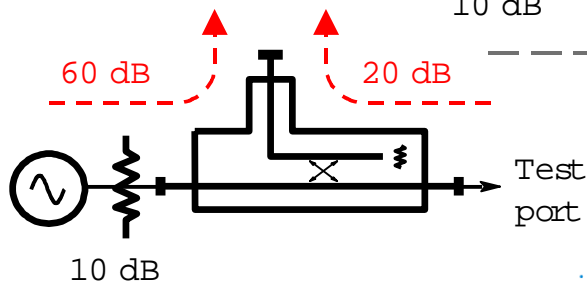

$$\text{Directivity} = 60 \text{ dB} - 20 \text{ dB} - 10 \text{ dB} = 30 \text{ dB}$$




One Method of Measuring Coupler Directivity

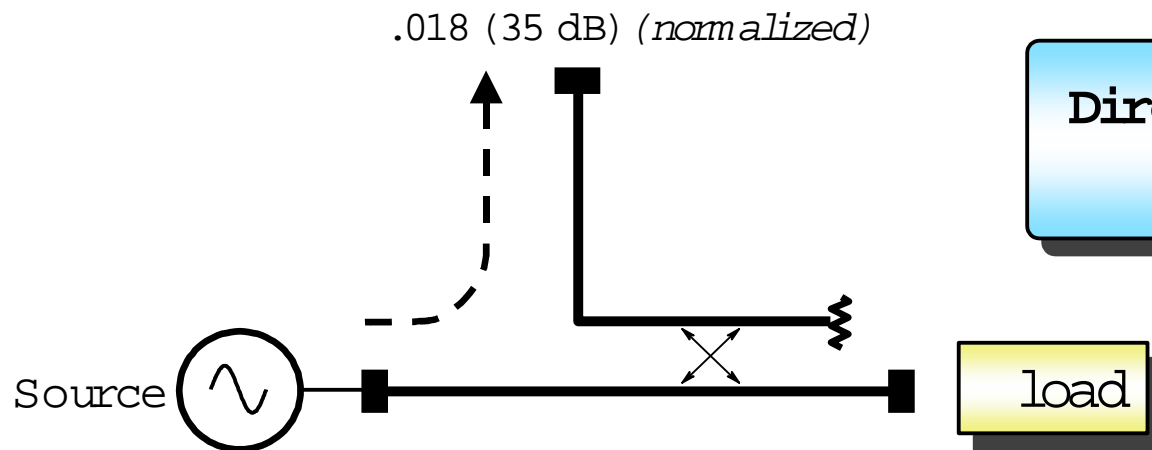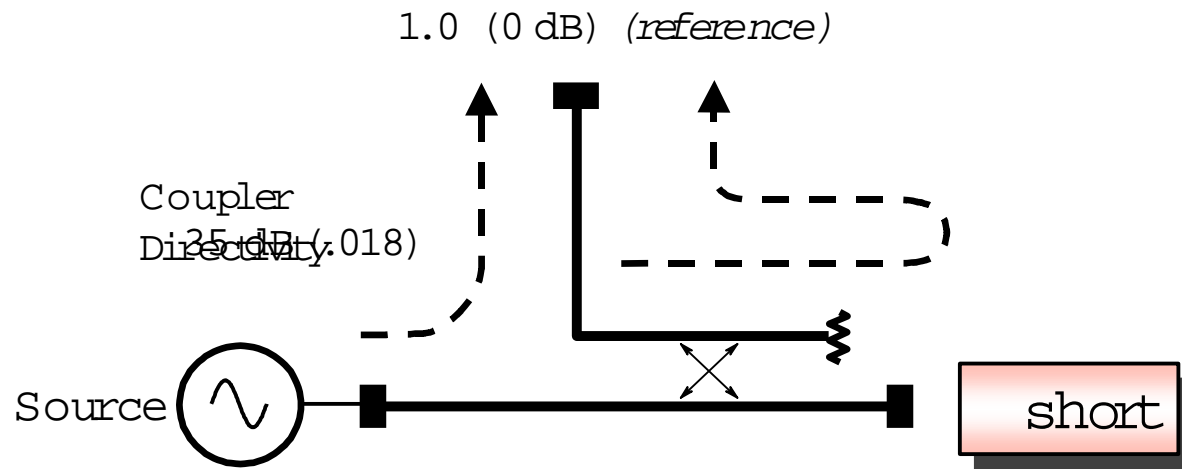

$$\begin{aligned}\text{Directivity} &= 35 \text{ dB} - 0 \text{ dB} \\ &= 35 \text{ dB}\end{aligned}$$

Assume perfect
load (no
reflection)



Directional Bridge

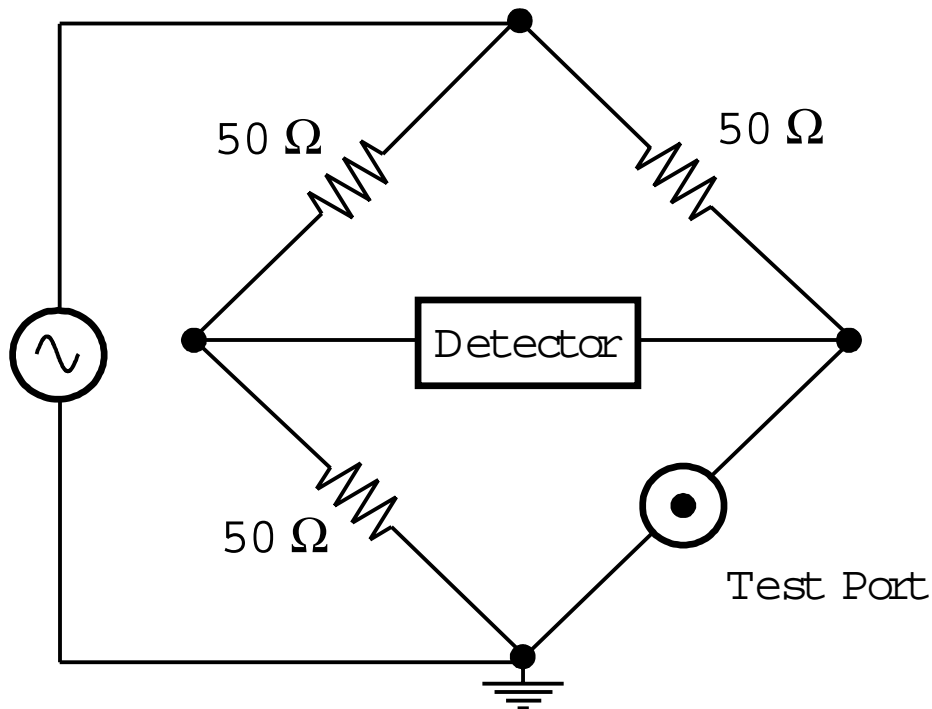


- 50-ohm load at test port balances the bridge — detector reads zero
- Non-50-ohm load imbalances bridge
- Measuring magnitude and phase of imbalance gives complex impedance
- "Directivity" is difference between maximum and minimum balance



NA Hardware: Front Ends, Mixers Versus Samplers

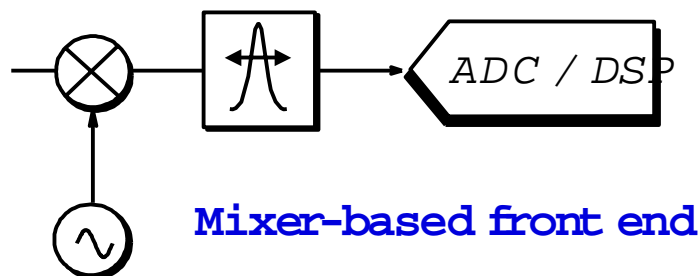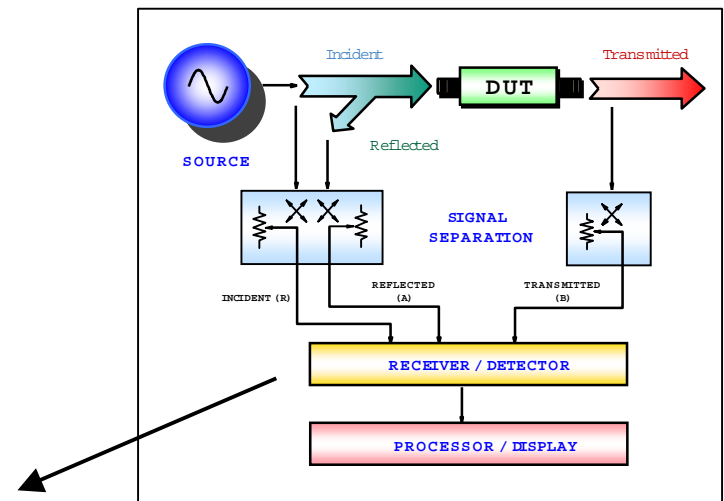


Sampler-based front end

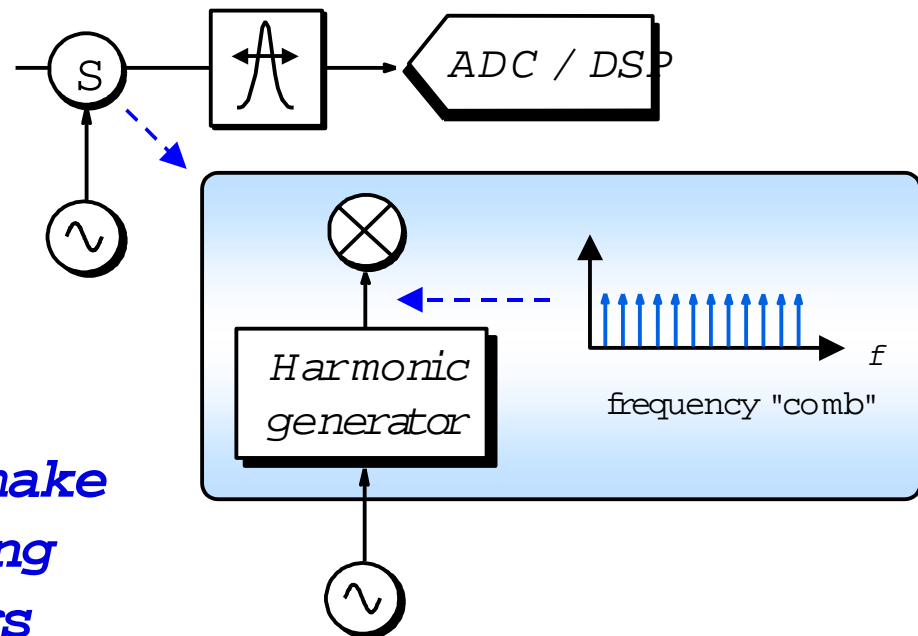

It is cheaper and easier to make broadband front ends using samplers instead of mixers




Three Versus Four-Receiver Analyzers

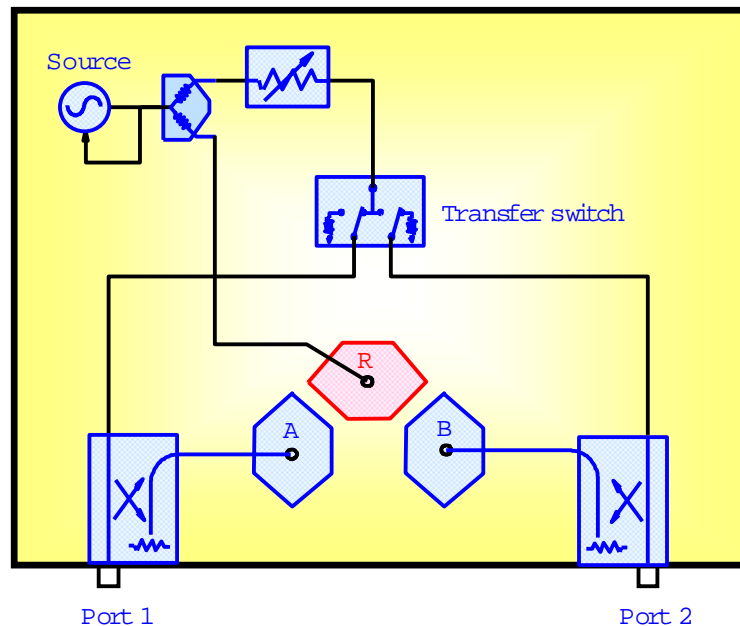

3 receivers

- more economical
- TRL*, LRM* cals only
- includes:
 - 8753ES
 - 8720ES (standard)

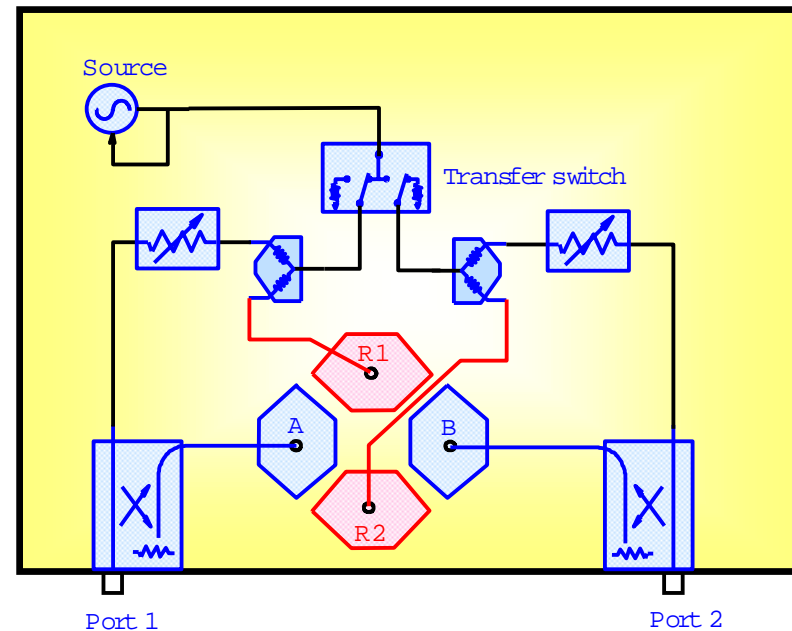


4 receivers

- more expensive
- true TRL, LRM cals
- includes:
 - 8720ES (option 400)
 - 8510C



Why Are Four Receivers Better Than Three?

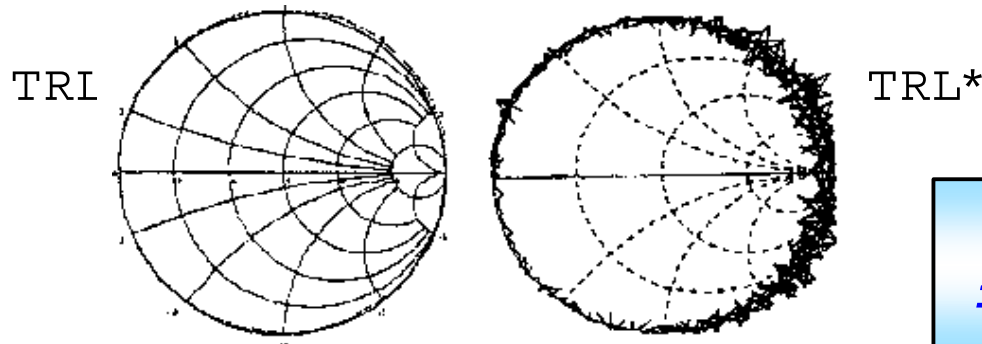

*8720ES Option 400 adds
fourth sampler, allowing full
TRL calibration*

- **TRL***
 - assumes the **source and load match** of a test port are **equal** (port symmetry between forward and reverse measurements)
 - this is only a fair assumption for three-receiver network analyzers
- **TRL**
 - four receivers are necessary to make the required measurements
 - TRL and TRL* use identical calibration standards
- **In noncoaxial applications**, TRL achieves **better source and load match correction** than TRL*
- **What about coaxial applications?**
 - **SOLT is usually the preferred calibration method**
 - coaxial TRL can be more accurate than SOLT, but not commonly used



Challenge Quiz

1. Can filters cause distortion in communications systems?

- A. Yes, due to impairment of phase and magnitude response
- B. Yes, due to nonlinear components such as ferrite inductors
- C. No, only active devices can cause distortion
- D. No, filters only cause linear phase shifts
- E. Both A and B above

2. Which statement about transmission lines is false?

- A. Useful for efficient transmission of RF power
- B. Requires termination in characteristic impedance for low VSWR
- C. Envelope voltage of RF signal is independent of position along line
- D. Used when wavelength of signal is small compared to length of line
- E. Can be realized in a variety of forms such as coaxial, waveguide, microstri

3. Which statement about narrowband detection is false?

- A. Is generally the cheapest way to detect microwave signals
- B. Provides much greater dynamic range than diode detection
- C. Uses variable-bandwidth IF filters to set analyzer noise floor
- D. Provides rejection of harmonic and spurious signals
- E. Uses mixers or samplers as downconverters



Challenge Quiz (continued)

- 4. Maximum dynamic range with narrowband detection is defined as:**
- A. Maximum receiver input power minus the stopband of the device under test
 - B. Maximum receiver input power minus the receiver's noise floor
 - C. Detector 1-dB-compression point minus the harmonic level of the source
 - D. Receiver damage level plus the maximum source output power
 - E. Maximum source output power minus the receiver's noise floor
- 5. With a T/R analyzer, the following error terms can be corrected:**
- A. Source match, load match, transmission tracking
 - B. Load match, reflection tracking, transmission tracking
 - C. Source match, reflection tracking, transmission tracking
 - D. Directivity, source match, load match
 - E. Directivity, reflection tracking, load match
- 6. Calibration(s) can remove which of the following types of measurement**
- A. Systematic and drift
 - B. Systematic and random
 - C. Random and drift
 - D. Repeatability and systematic
 - E. Repeatability and drift



Challenge Quiz (continued)

7. Which statement about TRL calibration is false?

- A. Is a type of two-port error correction
- B. Uses easily fabricated and characterized standards
- C. Most commonly used in noncoaxial environments
- D. Is not available on the 8720ES family of microwave network analyzers
- E. Has a special version for three-sampler network analyzers

8. For which component is it hardest to get accurate transmission and reflection measurements when using a T/R network analyzer?

- A. Amplifiers because output power causes receiver compression
- B. Cables because load match cannot be corrected
- C. Filter stopbands because of lack of dynamic range
- D. Mixers because of lack of broadband detectors
- E. Attenuators because source match cannot be corrected

9. Power sweeps are good for which measurements?

- A. Gain compression
- B. AM to PM conversion
- C. Saturated output power

Answers to Challenge Quiz

1. E

2. C

3. A

4. B

5. C

6. A

7. D

8. B

9. E